



(19) **United States**

(12) **Patent Application Publication**
Gubbini et al.

(10) **Pub. No.: US 2012/0022379 A1**

(43) **Pub. Date: Jan. 26, 2012**

(54) **ULTRASOUND PROBE**

Related U.S. Application Data

(75) Inventors: **Alessandro Gubbini**, State College, PA (US); **William R. Dreschel**, State College, PA (US)

(60) Provisional application No. 61/165,630, filed on Apr. 1, 2009.

Publication Classification

(73) Assignee: **ANALOGIC CORPORATION**, Peabody, MA (US)

(51) **Int. Cl.**
A61B 8/14 (2006.01)

(52) **U.S. Cl.** **600/461; 600/459**

(57) **ABSTRACT**


(21) Appl. No.: **13/256,447**

An ultrasound imaging probe (101) includes a communications interface (107), including one or more ports (200-205), corresponding to one or more different communication protocols, for communication with ultrasound consoles. The probe (101) also includes a controller (106) that configures the probe (101) for communication with an ultrasound console (102) over a port (200-205) based on a communication between the communications interface (107) and a communications interface (110) of the console (102).

(22) PCT Filed: **Jun. 24, 2009**

(86) PCT No.: **PCT/US2009/048374**

§ 371 (c)(1),
(2), (4) Date: **Sep. 14, 2011**

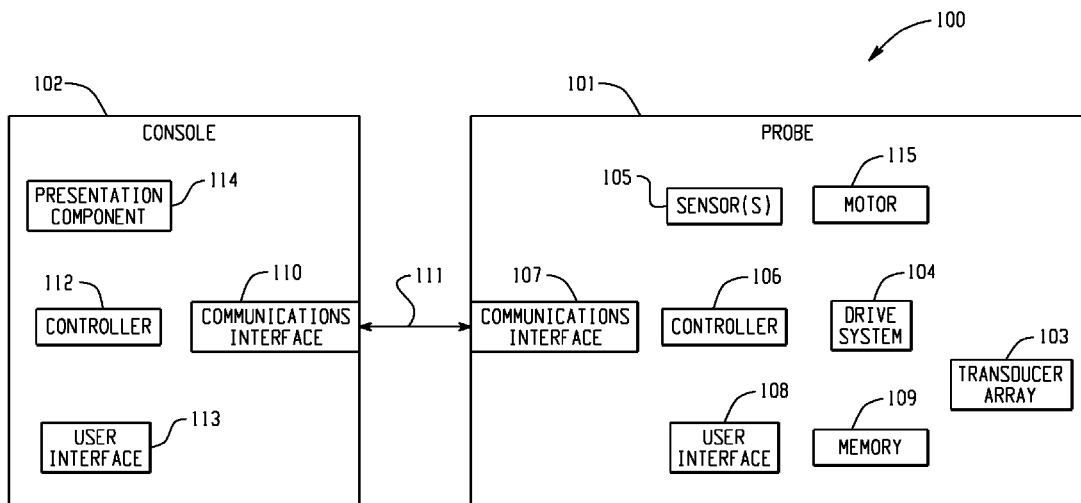

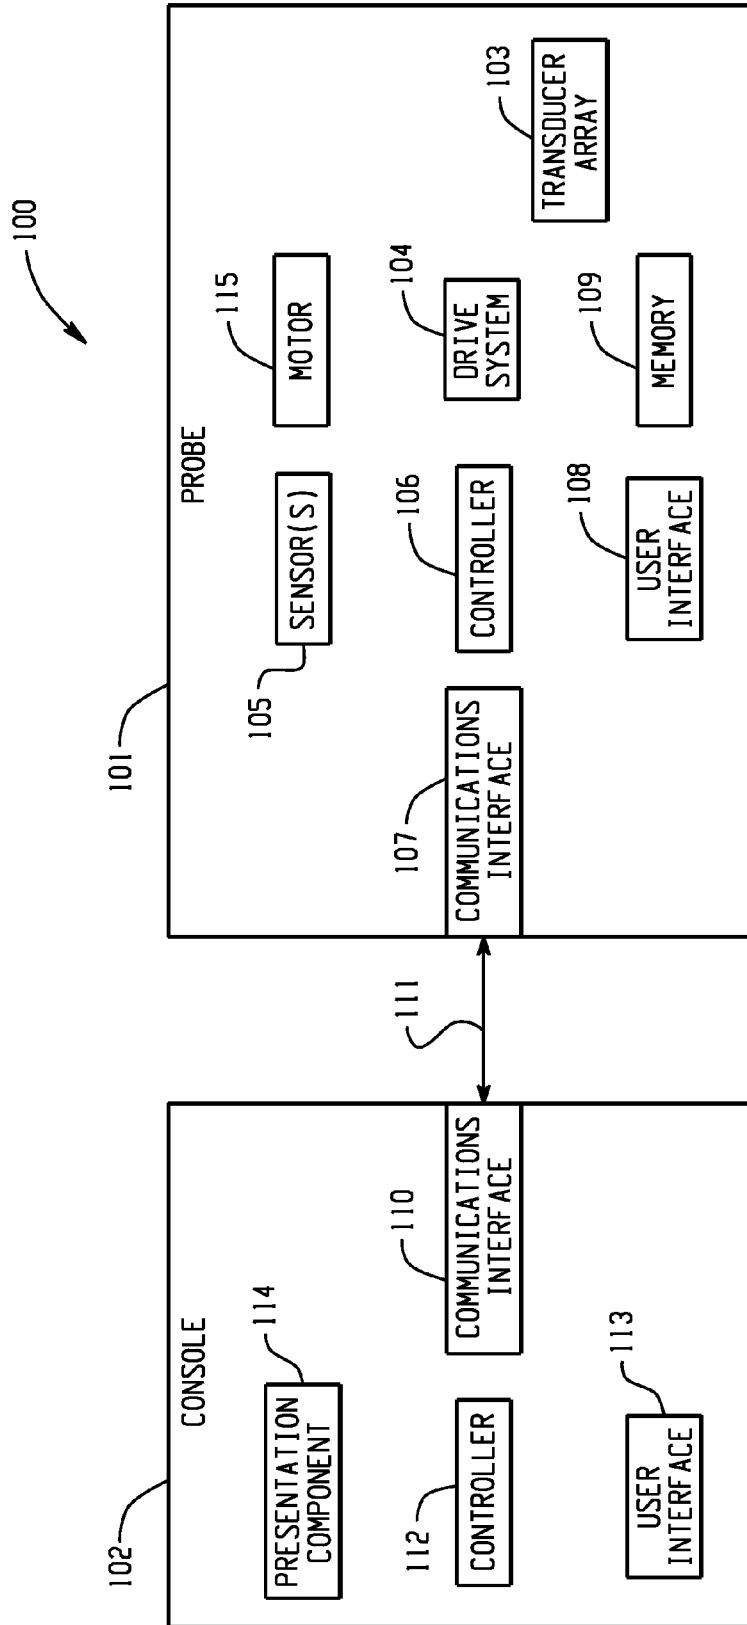


Fig. 1

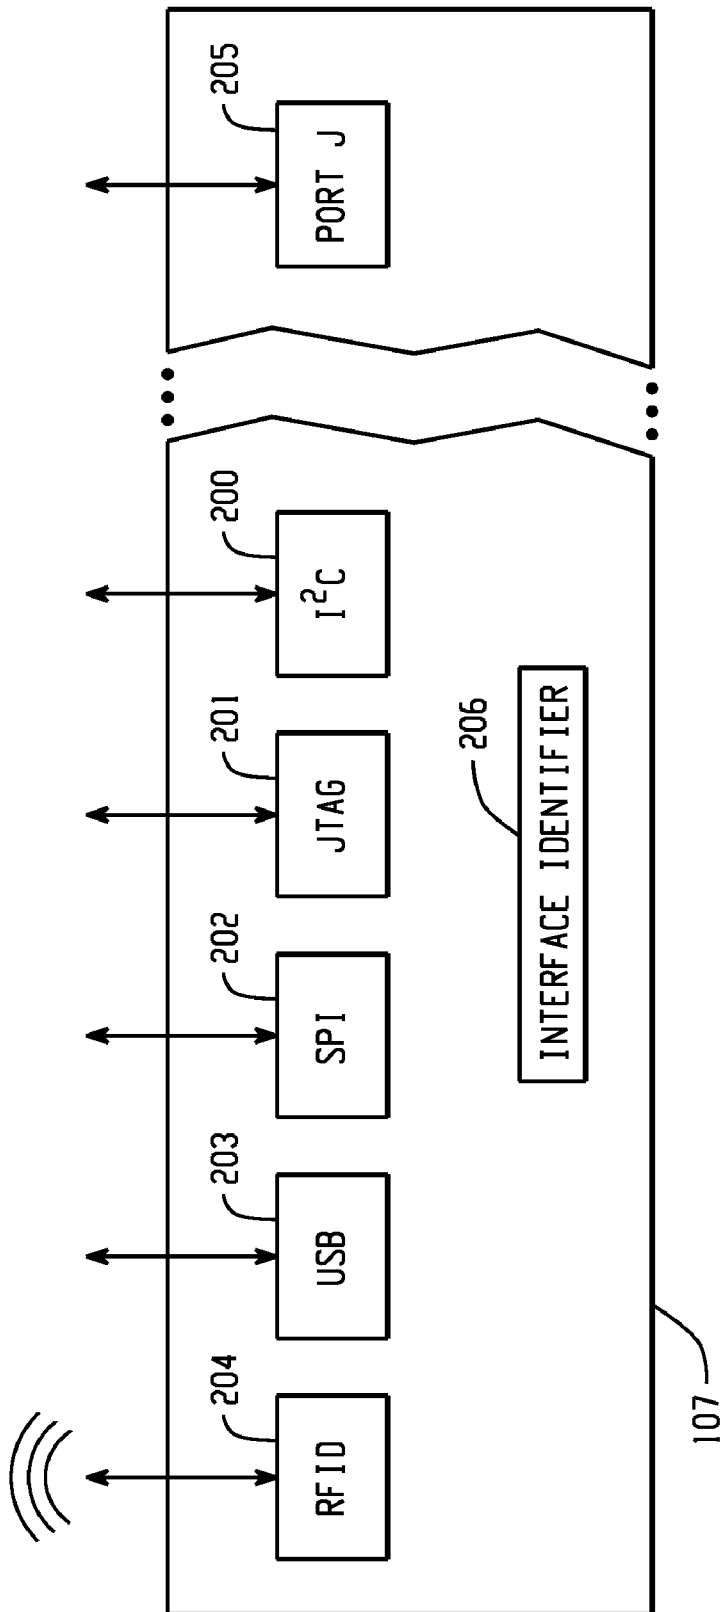


Fig. 2

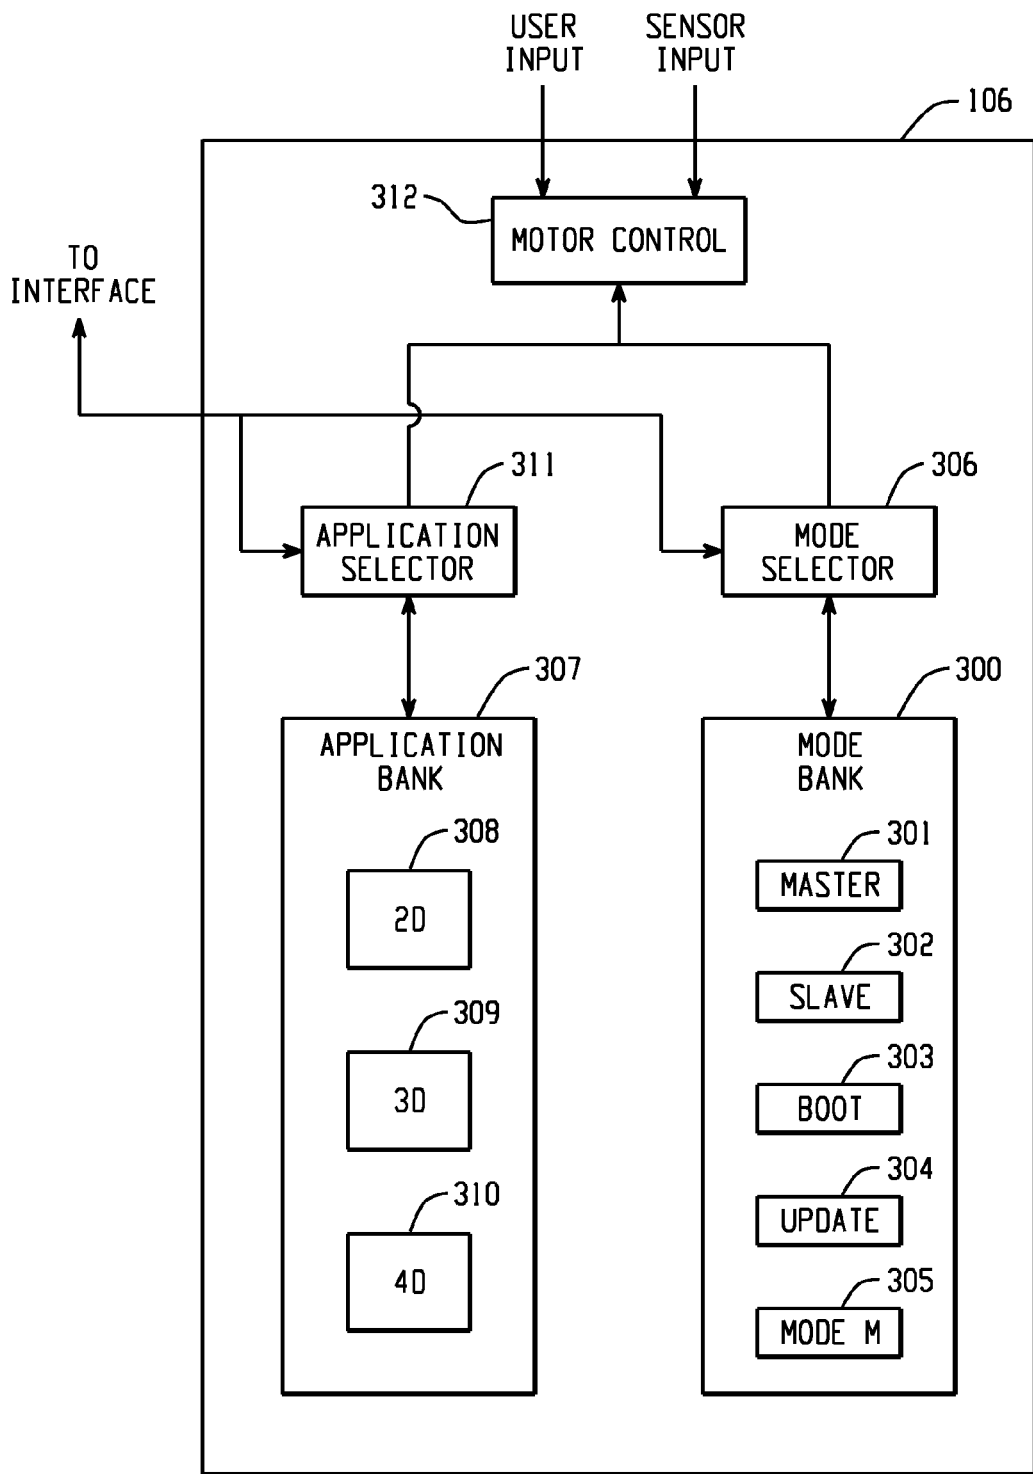


Fig. 3

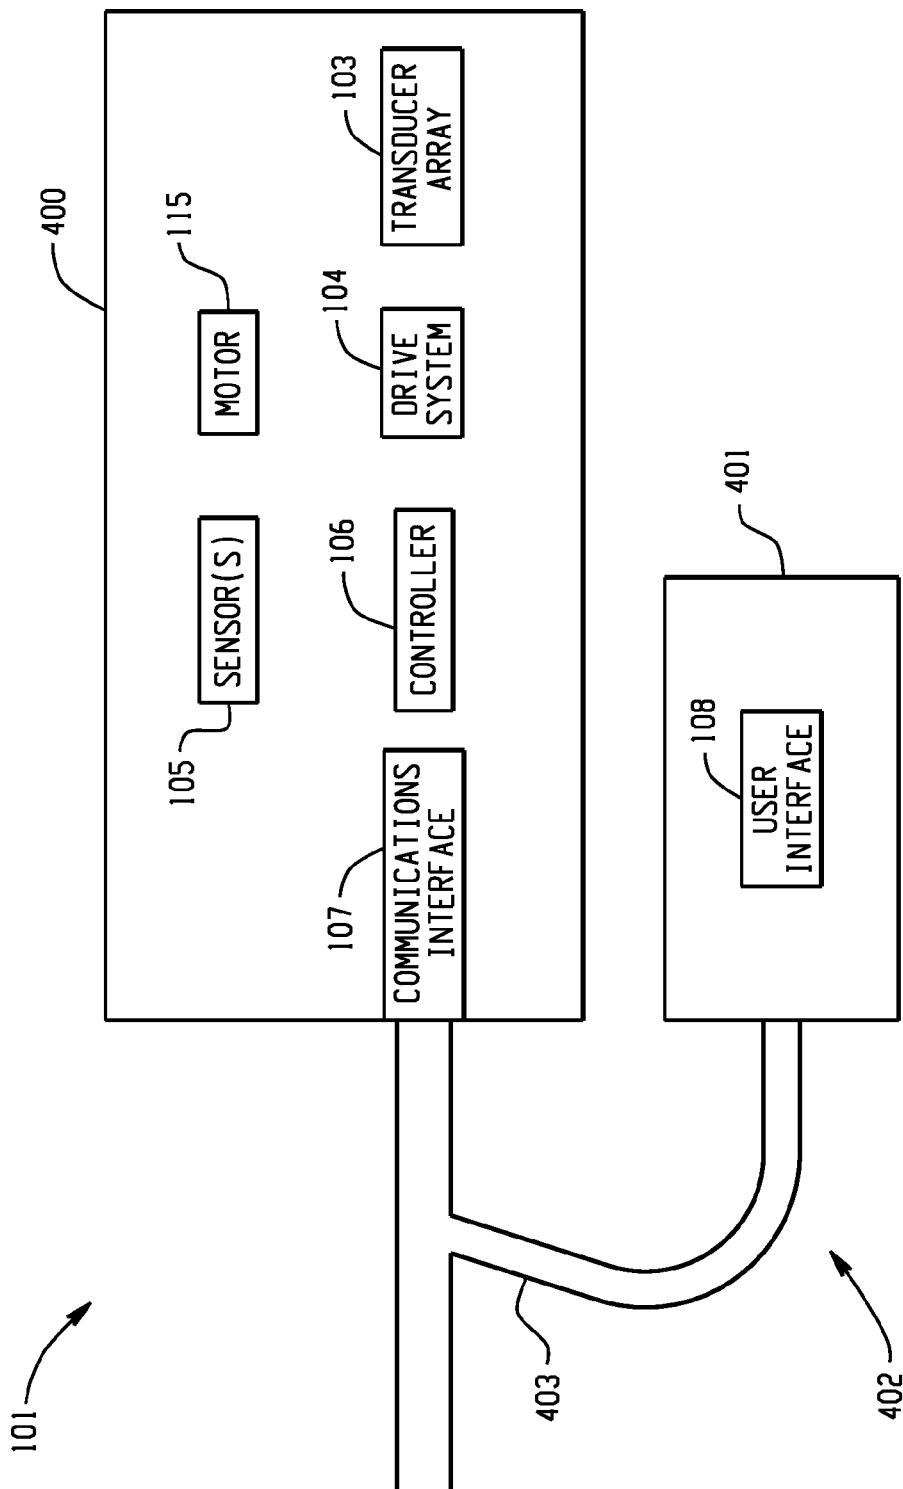


Fig. 4

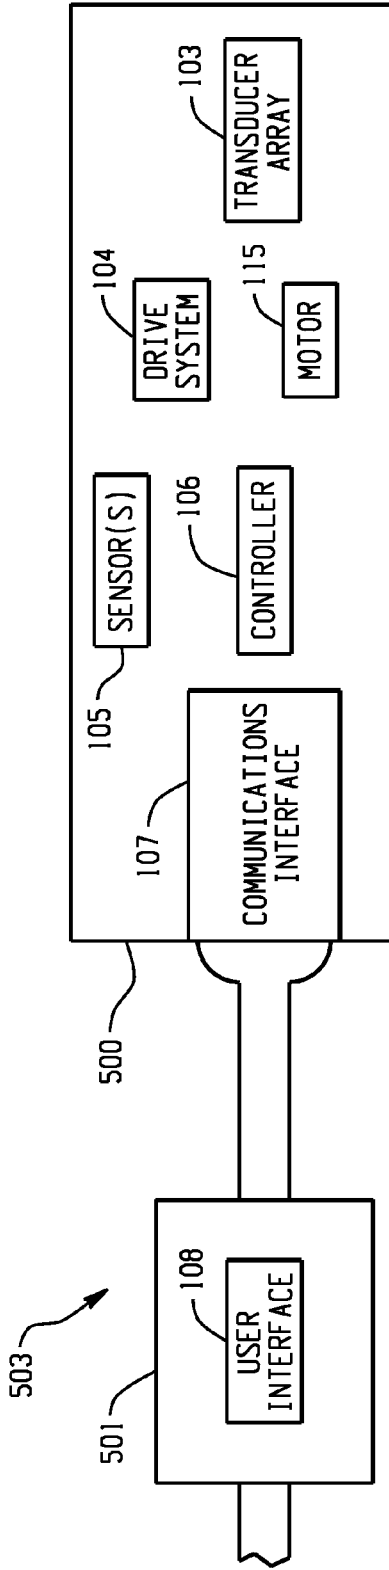


Fig. 5

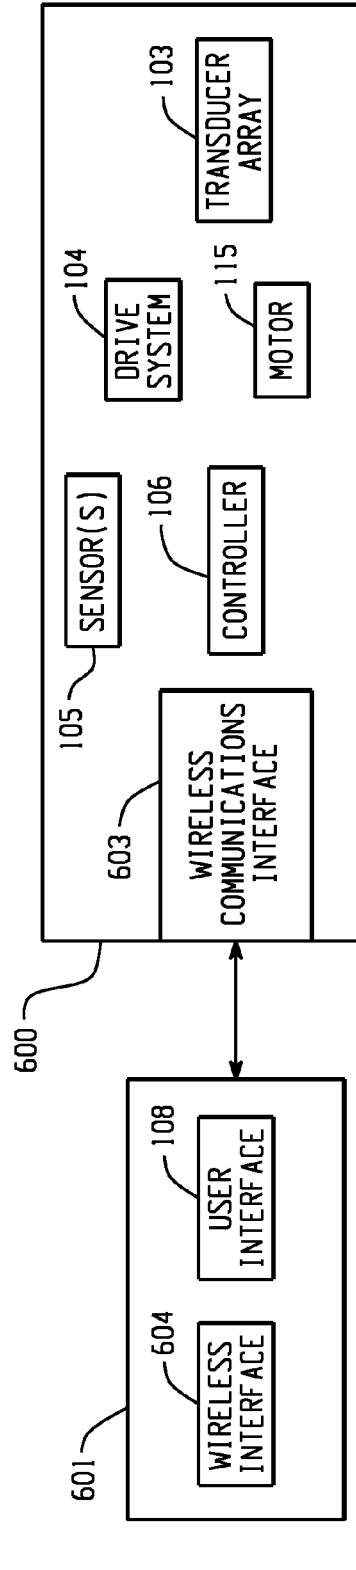


Fig. 6

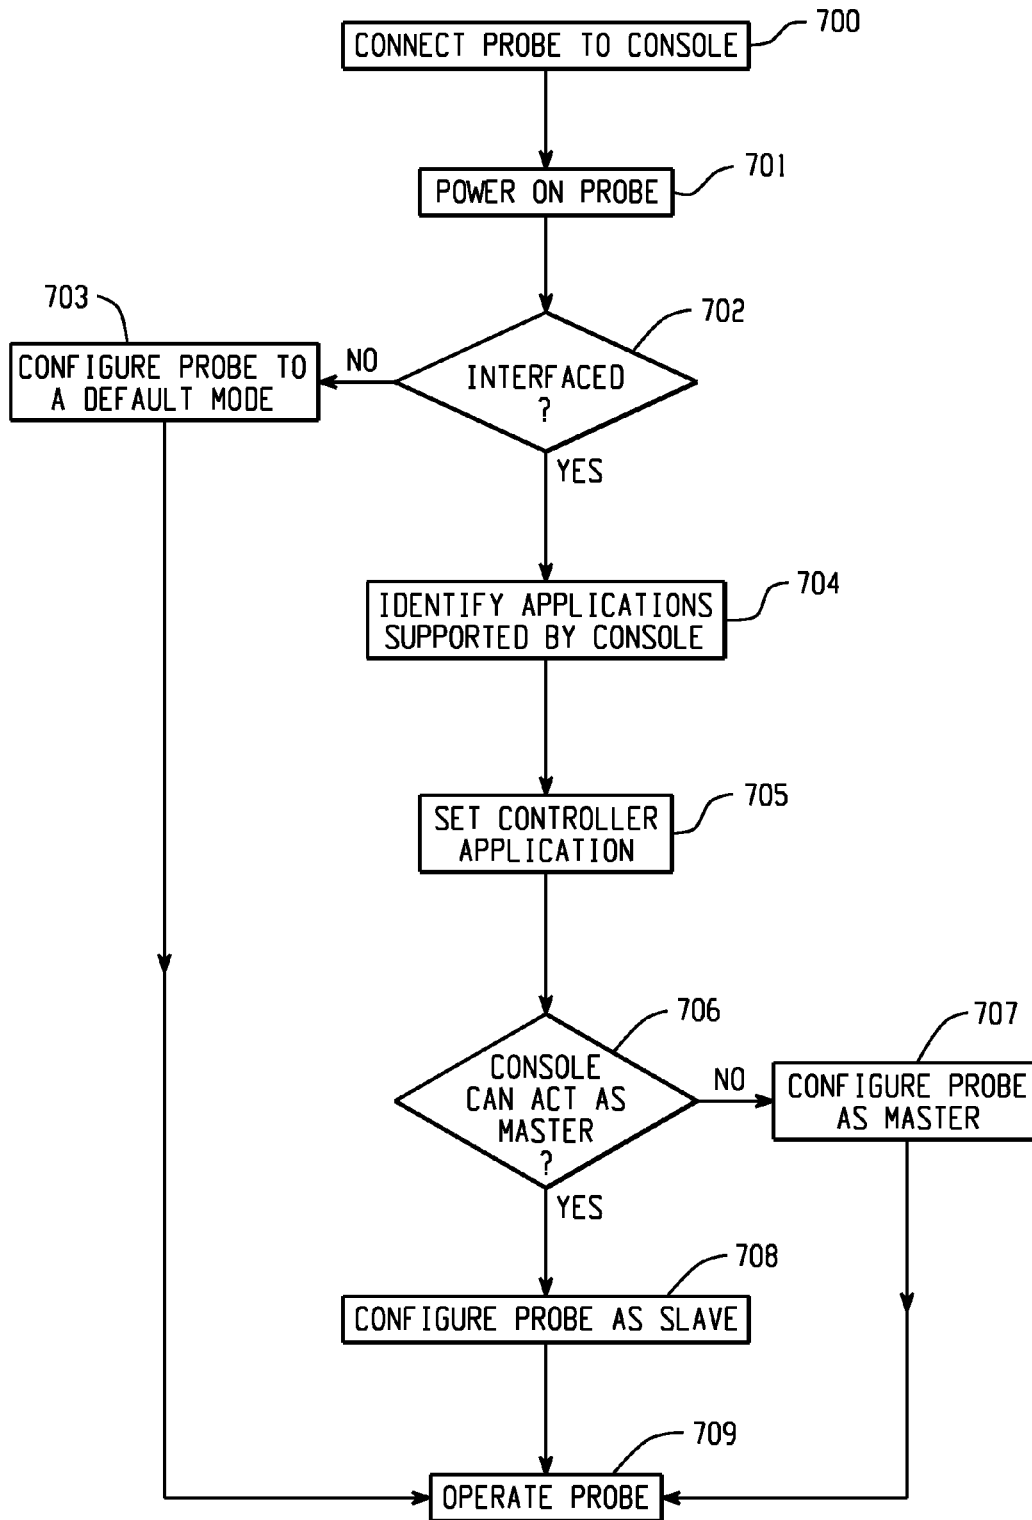


Fig. 7

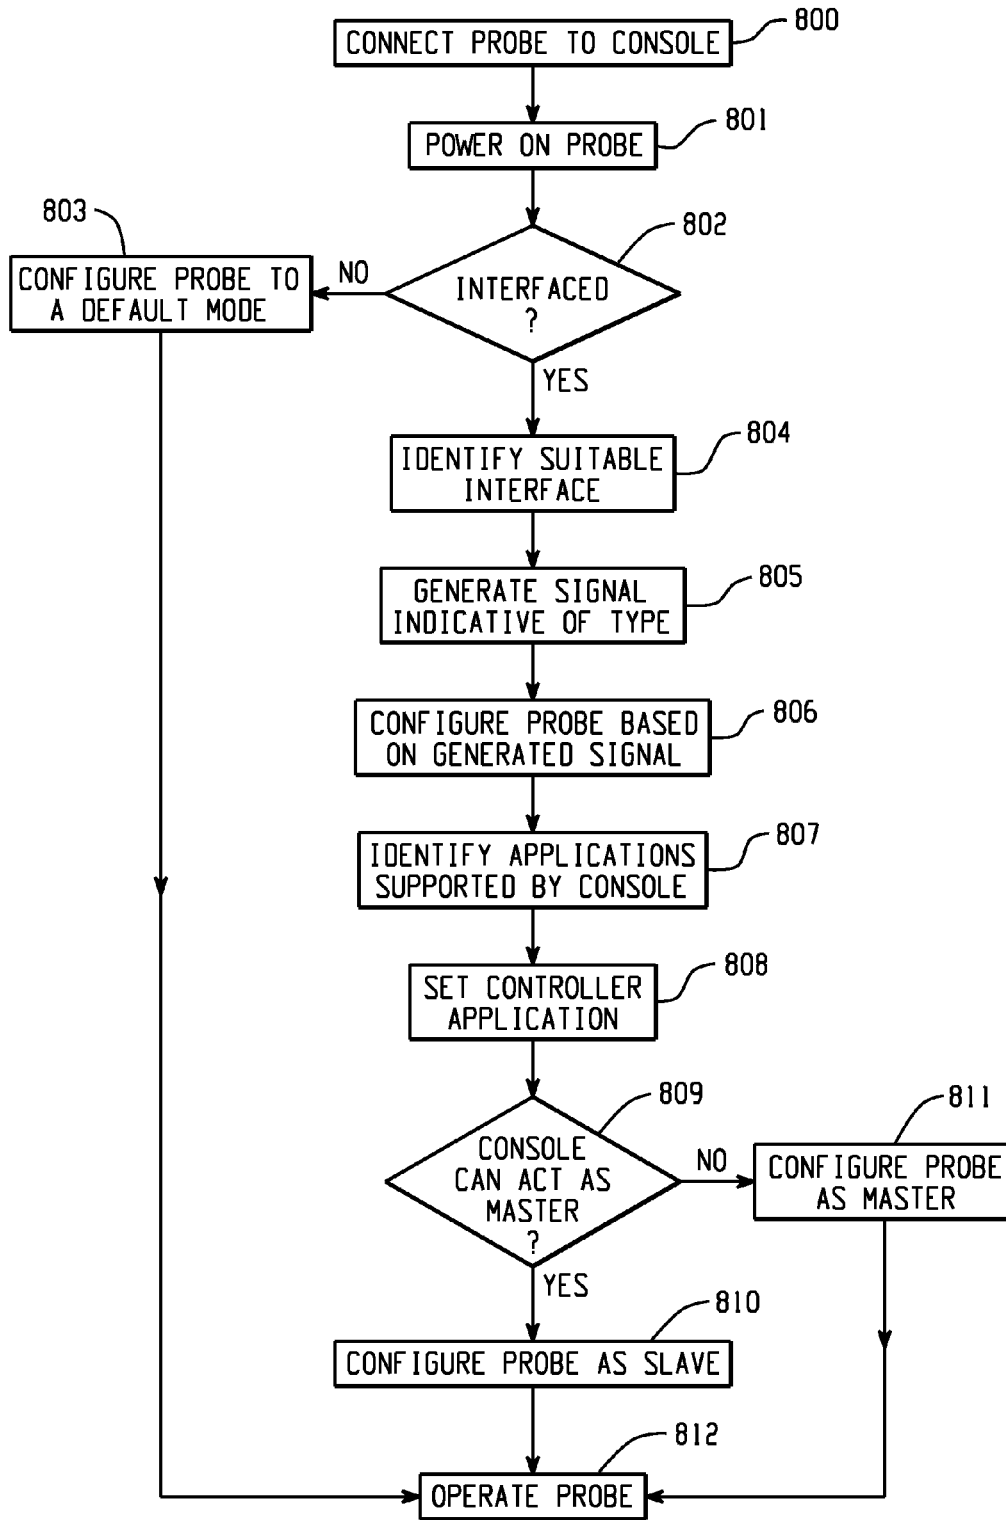


Fig. 8

ULTRASOUND PROBE

CROSS REFERENCE TO RELATED APPLICATIONS

[0001] This application claims the benefit of priority of provisional patent application Ser. No. 61/165,630, filed on Apr. 1, 2009, confirmation number 4363, and entitled "ULTRASOUND PROBE," which is incorporated herein in its entirety by reference.

TECHNICAL FIELD

[0002] The following generally relates to ultrasound probes and more particularly to ultrasound probes configured for multi-dimensional imaging.

BACKGROUND

[0003] An ultrasound imaging probe generally includes one or more transducer arrays, affixed to a distal end of a mechanical device or a handle, and can be used for imaging of anatomical structures or organs. Volumetric imaging can be performed by using two-dimensional transducer arrays with no moving parts or by electromechanically moving a one-dimensional transducer array within the probe. Volumetric imaging has been used to visualize three-dimensional structures within the human body such as the kidneys, the uterus, a fetus, etc.

[0004] For patient imaging, the probe (and hence the transducer elements) is moved on the surface of the body over the structure of interest. The transducer generates a signal that traverses skin, subcutaneous fat, and/or bone material, reflects off the structure of interest, and is received back and detected at the transducer. The detected information is used to generate an image of the structure of interest. With other ultrasound applications (e.g., transabdominal, endovaginal, and endorectal), the transducer is positioned in and moved within a body cavity to image anatomical structures.

[0005] Unfortunately, some ultrasound probes are controllable only through ultrasound imaging systems and configured such that they only work with specific ultrasound imaging systems. As a consequence, a probe configured for multi-dimensional imaging may not be able to be used for multi-dimensional imaging when employed with an ultrasound imaging system that does not support multi-dimensional imaging applications. In addition, a probe configured with a particular interface may not be able to be used with a console that does not have a complementary interface. In addition, a console may lack suitable circuitry for controlling various components of a probe in communication therewith.

SUMMARY OF THE INVENTION

[0006] Aspects of the application address the above matters, and others.

[0007] In one aspect, an ultrasound imaging probe includes a communications interface with one port or a plurality of ports corresponding to one or more different communication protocols for communication with ultrasound consoles. The probe also includes a controller that configures the probe for communication with an ultrasound console over a port based on a communication between the communications interface and a communications interface of the console.

[0008] In a further aspect, an ultrasound probe includes a transducer array, an electromechanical drive system, a motor,

and a controller that controls the drive system and motor to drive the transducer array to at least one of translate or wobble.

[0009] In a further aspect, a method includes identifying a type of communications interface of an ultrasound console in communication with an ultrasound imaging probe and selecting a communications port of the probe for communication between the probe and the console based on the identified type of communications interface.

[0010] In a further aspect, an ultrasound probe for three and/or four dimensional ultrasound applications includes a controller that configures the probe for use with a console that does not support three and/or four-dimensional ultrasound applications.

[0011] Those skilled in the art will recognize still other aspects of the present application upon reading and understanding the attached description.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] FIG. 1 illustrates an example probe and console of an imaging system.

[0013] FIG. 2 illustrates an example communications interface of a probe.

[0014] FIG. 3 illustrates an example probe controller logic.

[0015] FIG. 4 illustrates an example probe with user controls in a dongle.

[0016] FIG. 5 illustrates an example probe with user controls in a cable.

[0017] FIG. 6 illustrates an example probe with wireless control.

[0018] FIG. 7 illustrates one method for using an example probe and console of an imaging system.

[0019] FIG. 8 illustrates a second method for using an example probe and console of an imaging system.

DETAILED DESCRIPTION

[0020] FIG. 1 depicts an ultrasound imaging system **100** including a probe **101** and a console **102**. The probe **101** is capable of multi-dimensional applications such as two, three and four-dimensional applications and includes a movable transducer array **103** having one or more transducer elements that transmit and detect signals. Non-limiting examples of suitable transducer elements include piezoceramic, MEMS and/or other transducer elements.

[0021] An electromechanical drive system **104** moves and/or orients the movable transducer array **103** through a motor **115**. In one instance, this includes converting rotational motion of the motor **115** into translational, rotational and/or wobbling movement of the ultrasound transducer array **103**. Suitable motors **115** may include but are not limited to a stepper motor, a DC motor, an ultrasonic motor, a piezoelectric motor, an electromagnetic motor, and/or other motor. The illustrated drive system **104** and motor **115** are configured to drive the transducer array **103** alternatively based on one or more predetermined and/or programmable movement patterns.

[0022] One or more sensors **105** sense information about the operating conditions of the probe **101**. Suitable sensors include an optical or magnetic encoder that senses probe orientation; a temperature sensor that detects a temperature of the drive system **104**, the transducer array **103** or one or more

other components of the probe **101**; a needle guide sensor that senses a needle guide coupled to the probe **101**, and/or other sensor.

[0023] A controller **106** controls the drive system **104** and hence position of the transducer array **103**. In one instance, the controller **106** controls the drive system **104** based on a mode of operation including a master, a slave, a self-booting, software loading, and/or other mode of operation and an application mode such as a two, three or four dimensional application. As described in greater detail below, the controller **106** identifies a suitable mode of operation and application mode based on a communication with the console **102**. The controller **106** may also use the information sensed by the sensors **105** and/or user input to identify the mode and application.

[0024] A communications interface **107** is configured to receive and transmit information between the probe **101** and the console **102** and/or other device. As described in greater detail below, the interface **107** may be configured with a single communications port or with a plurality of communication ports for communicating with one or more different consoles **102** supporting different communication protocols. The interface **107** includes an analog portion for communication with analog components of the probe **101** and/or a digital portion for communication with digital components of the probe **101**. For example, where the transducer array **103** is an analog transducer array, the analog portion is used to communicate with the transducer array **103**, and where the drive system **104** is a digital drive system, the digital portion is used to communicate with the drive system **104**.

[0025] A user interface **108** accepts user input and presents operational and/or application information in a human readable format. Examples of input include signals representing a particular mode of operation and/or application mode. In one embodiment, the user interface **108** accepts user input through a touch pad and/or predetermined control buttons. Additionally or alternatively, the user interface **108** includes an audio input for accepting voice commands or other audio information.

[0026] Memory **109** provides storage for data and/or other information, for example, configuration and/or imaging data from the transducer array **103** and/or data from the ultrasound console **102**. The memory **109** may include software and/or firmware uploaded by a user. Such software and/or firmware may make the probe **101** specific to the user and/or supporting equipment.

[0027] It is to be appreciated that by incorporating the controller **106** in the probe **101** and allowing the configuration of different communication providing one or a plurality of different communication ports by the interface **107** allows the probe **101** to be used with essentially any console **102**. For example, where the controller **106** is omitted from the probe **101**, the probe **101** may only be employed with a console **102** having control circuitry compatible with or able to drive the drive system **104** and the motor **115** of the probe **101**. In another example, where the communication interface **107** only supports a single type of port, the probe **101** may only be employed with a console **102** supporting that type of port.

[0028] The console **102** includes a communication interface **110**. The probe **101** interfaces with the console **102** through the communication interface **110** over a channel **111**, which may be a wired or wireless channel. The console **102** also includes a controller **112**, which can send signals indicative of a selected mode of operation and/or application mode

to the probe **101**. A user interface **113** allows a user to communicate with the probe **101** through the console **102**. A presentation component **114** presents image data.

[0029] With reference to FIGS. **1** and **2**, FIG. **2** illustrates an example of the communications interface **107** with a plurality of communication ports.

[0030] In the illustrated example, the communications interface **107** includes an Inter-Integrated Circuit (I²C) port **200**, which generally is a multi-master serial bus used to attach low-speed peripherals to an embedded system. The communications interface **107** further includes a Joint Action Test Group (JTAG) port **201**, which is generally a test access port for debugging and probing printed circuit boards.

[0031] The communications interface **107** also includes a Serial Peripheral Interface (SPI) port **204**, which generally is a synchronous serial data link that allows a single master device. The communications interface **107** further includes a Universal Serial Bus (USB) port **203**, which is a standardized interface socket that generally allows connection of peripheral devices.

[0032] The communications interface **107** further includes a wireless port such as a Radio Frequency Identification (RFID) port **203**. The communications interface **107** may also include one or more other ports (PORT J) **205**.

[0033] An interface identifier **206** identifies the port in communication with the console **102** and generates a signal indicative thereof. The signal is provided to the controller **106**, which configures the probe **101** for communication over the identified port.

[0034] With reference to FIGS. **1** and **3**, FIG. **3** illustrates an example of the controller **106**.

[0035] The controller **106** includes a mode bank **300** with one or more predetermined modes such as a master mode **301**, a slave mode **302**, a boot mode **303**, an update mode **304**, and one or more other modes **305**. A mode selector **306** selects a mode of operation from the mode bank **300** based on various information.

[0036] The controller **106** also includes an application bank **307** with one or more predetermined application modes such as a two-dimensional mode **308**, a three-dimensional mode **309**, and a four-dimensional mode **310**. An application selector **311** selects an application mode from the application bank **307** based on various information.

[0037] As described herein, the controller **106** configures the probe **101** based on a selected mode of operation, a selected application mode, information sensed by the sensor (s) **105**, and a user input. In one instance, the controller **106** recognizes that the console does not support three or four-dimensional applications and configures the probe **101** so that the probe **101** can be used for three or four-dimensional applications using the user interface **108** of the probe **101**. In this instance, the multi-dimensional imaging data may be stored in a memory **109** for subsequent retrieval.

[0038] A motion controller **312** generates a control signal for the drive system **104** based on the one or more of the selected operation mode, application mode, user input and/or sensor input. The control signal is indicative of movement and/or orientation of the transducer array **103**.

[0039] FIGS. **4**, **5**, and **6** depict alternative embodiments of the probe **101**.

[0040] Initially referring to FIG. **4**, the probe **101** includes first and second portions **400** and **401**. The first portion **400** includes the transducer array **103**, the drive system **104**, the motor **115**, the sensors **105**, the controller **106**, and the inter-

face 107. The second portion 401 includes the user interface 108. The second portion 401 is part of dongle 402 and is connected to the first portion 400 through a connection 403, which can be a wired and/or wireless connection.

[0041] Turning to FIG. 5, the probe 101 includes first and second portions 500 and 501. The first portion 500 includes the transducer array 103, the drive system 104, the motor 115, the sensors 105, the controller 106 and the interface 107, and the second portion 501 includes the user interface 103. In this embodiment, the second portion 501 is integrated in or part of a cable 503, which is used to connect the probe 101 to the console 102.

[0042] In FIG. 6, the probe 101 includes first and second portions 600 and 601. The first portion 600 includes the transducer array 103, the drive system 104, the motor 115, the sensors 105, the controller 106, and a wireless interface 603. The second portion 601 includes the user interface 108 and a wireless interface 604. In this embodiment, the first and second portions 600 and 601 communicate with each other through the wireless interfaces 603 and 604.

[0043] In another embodiment, the controller 106 is located within a handle shield, which is formed as an external probe covering which acts also as a ground plane and heat distributor. In yet another embodiment, the controller 106 is incorporated within a handle in which in multiple components can be interchanged to provide a user or application specific probe. In still another embodiment, the controller 106 is part of independent circuitry which may be coupled to and employed with a plurality of different ultrasound probes, in conjunction with multiple different ultrasound imaging systems.

[0044] FIG. 7 illustrates a method in connection with FIGS. 1-3 where the probe 101 is configured to communicate with the console 102 through a single interface.

[0045] At 700, the probe 101 is connected to the console 102.

[0046] At 701, the probe 101 is powered on. This can be achieved by activating a power switch or toggle of the user interface 108.

[0047] At 702, the probe 101 attempts communications with the console 102.

[0048] At 703, if the communication fails, the controller 106 places the probe 101 in a default mode, such as, the slave mode 302. In this mode, an application is selected and the probe 101 is controlled through the console 102.

[0049] At 704, if the communications is successful, the controller 106 identifies applications (two, three and/or four dimensions) supported by the console 102.

[0050] At 705, the controller 106 configures itself based on the identified supported applications. This includes allowing the probe 101 to be operated by the console 102 based on the applications supported by the console 102 and/or operated by the probe 101, including using applications that are not supported by the console 102.

[0051] At 706, the controller 106 determines whether the console 102 can act as a master device. At 707, if not, the probe 101 configures the probe 101 as a master device.

[0052] At 708, otherwise, the controller 106 configures the probe 101 as a slave device.

[0053] At 709, the probe 101 is employed based on user input to the probe 101, the console 102, and/or information sensed by the sensors 105.

[0054] FIG. 8 illustrates a method in connection with FIGS. 1-3 where the probe 101 is configured to communicate with the console 102 through one or a plurality of different interfaces.

[0055] At 800, the probe 101 is connected to the console 102.

[0056] At 801, the probe 101 is powered on. This can be achieved by activating a power switch of the user interface 108.

[0057] At 802, the probe 101 attempts communications with the console 102.

[0058] At 803, if the communication fails, the controller 106 places the probe 101 in a default mode such as the master mode 301. In this mode, an application is selected and the probe 101 is controlled through the user interface 108.

[0059] At 804, if the communications is successful, the interface identifier 206 identifies the type of interface through which the probe 101 and console 102 are connected.

[0060] At 805, the interface identifier 206 generates a signal indicative of the identified type of interface.

[0061] At 806, the controller 106 configures the probe 101 to communicate based on the identified type of interface.

[0062] At 807, the controller 106 identifies applications (two, three and/or four dimensions) supported by the console 102.

[0063] At 808, the controller 106 configures itself based on the identified supported applications. This includes allowing the probe 101 to be operated by the console 102 based on the applications supported by the console 102 and/or operated by the probe 101, including using applications that are not supported by the console 102.

[0064] At 809, the controller 106 determines whether the console 102 can act as a master device. At 810, if so, the probe 101 configures the probe 101 as a slave device. Of course, the user can override this setting and/or the default settings may be that the probe 101 configures itself as the master device.

[0065] At 811, otherwise, the controller 106 configures the probe 101 as the master device.

[0066] At 812, the probe 101 is employed based on user input to the probe 101, the console 102, and/or information sensed by the sensors 105. Obtained data may be stored within a memory 109 of the probe 101 or transferred to the ultrasound console 102 or transmitted to other computing devices.

[0067] The application has been described with reference to various embodiments. Modifications and alterations will occur to others upon reading the application. It is intended that the invention be construed as including all such modifications and alterations, including insofar as they come within the scope of the appended claims and the equivalents thereof.

1. An ultrasound imaging probe, comprising:
 - a user interface;
 - a communications interface, including one or more ports, corresponding to one or more different communication protocols, for communication with ultrasound consoles; and
 - a controller that configures the probe for communication with an ultrasound console over a port based on a communication between the communications interface and a communications interface of the console, and an application selector that identifies application modes supported by the console, wherein the controller configures the probe based on an identified supported application, and

wherein the controller recognizes the console does not support three or four-dimensional applications and configures the probe for three or four-dimensional applications using the user interface of the probe.

2. The probe of claim 1, further comprising:
 - a transducer array;
 - an electromechanical drive system; and
 - a motor, wherein controller controls the drive system and the motor to at least one of translate or wobble the transducer array.
3. The probe of claim 2, wherein the console does not include circuitry for controlling the drive system and the motor.
4. The probe of claim 1, wherein the one or more ports includes at least one of an Inter-Integrated Circuit port, a Joint Action Test Group port, a Serial Peripheral Interface port, a Universal Serial Bus port, and a Radio Frequency Identification port.
5. The ultrasound probe of claim 1, wherein the communication identifies the communications interface of the console.
6. (canceled)
7. The probe of claim 1, wherein the controller configures the probe to a default operation and/or application mode when the probe is not in communication with the console.
8. The probe of claim 1, wherein the probe is configured for three and/or four-dimensional applications.
9. The probe of claim 1, wherein the probe is a master device and the console is a slave device.
10. The probe of claim 1, wherein the probe is a slave device and the console is a master device.
11. (canceled)
12. The probe (101) of claim 2, wherein the electromechanical drive system is housed in a portion of the probe housing the motor.
13. (canceled)
14. The probe of claim 1, wherein the controller configures the probe for default operation.
15. (canceled)
16. The probe of claim 1, further comprising at least one sensor, wherein the controller configures the probe based on information sensed by the at least one sensor.
17. The probe of claim 16, wherein the at least one sensor includes one or more of an optical and/or magnetic encoder that determines an orientation of the probe, a temperature sensor that determines a temperature of a component of the probe, and a needle guide sensor that senses a needle guide bracket mounted to the probe.
18. (canceled)
19. (canceled)
20. The ultrasound probe of claim 11, further comprising: a communications interface, including one or more ports, corresponding to one or more different communication protocols, for communication with ultrasound consoles, wherein the controller configures the probe for communication with

an ultrasound console over a port based on a communication between the communications interface and a communications interface of the console.

21. A method, comprising:
 - configuring a probe for communication with an ultrasound console over a port based on a communication between a communications interface of the probe and a communications interface of the console,
 - wherein the communications interface includes one or more ports that correspond to one or more different communication protocols for communication with ultrasound consoles,
 - identifying, via an application selector of the probe, application modes supported by the console; and
 - configuring, via a controller of the probe, the probe based on an identified supported application,
 wherein the controller recognizes the ultrasound console does not support three or four-dimensional applications and configures the probe for three or four-dimensional applications using an user interface of the probe.
- 22-28. (canceled)
29. A method, comprising:
 - sending, via an ultrasound probe, a communication to an ultrasound console over a connection there between;
 - identifying, via an application selector of the probe, applications supported by the console; and
 - configuring the probe, via a controller of the probe, based on the identified supported applications.
30. The method of claim 29, further comprising:
 - placing, via a controller of the probe, the probe in a default mode in response to the communication failing.
31. The method of claim 29, further comprising:
 - determining, via the controller of the probe, if the console can act as a master device;
 - configuring, via the controller of the probe, the probe as the master device and the console as a slave device, in response to determining the console cannot act as a master device; and
 - configuring, via the controller of the probe, the probe as a slave device and the console as a master device, in response to determining the console can act as a master device.
32. The method of claim 29, wherein the controller recognizes the ultrasound console does not support three or four-dimensional applications and configures the probe for three or four-dimensional applications under control of the probe.
33. The method of claim 29, further comprising:
 - prior to identifying the applications supported by the console, identifying, via an interface identifier of the probe, a type of interface through which the probe and console are connected in response to the communication being successful; and
 - configuring the probe, via the controller of the probe, to communicate based on the identified type of interface.

* * * * *