

(19)



(11)

EP 3 811 849 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention of the grant of the patent:
27.12.2023 Bulletin 2023/52

(51) International Patent Classification (IPC):
A61B 3/028 ^(2006.01) **A61B 3/00** ^(2006.01)
G02C 7/02 ^(2006.01)

(21) Application number: **19306384.9**

(52) Cooperative Patent Classification (CPC):
A61B 3/028; A61B 3/0025

(22) Date of filing: **24.10.2019**

(54) **METHOD AND SYSTEM FOR DETERMINING A PRESCRIPTION FOR AN EYE OF A PERSON**
VERFAHREN UND SYSTEM ZUR BESTIMMUNG EINES REZEPTS FÜR EIN AUGE EINER PERSON
PROCÉDÉ ET SYSTÈME POUR DÉTERMINER UNE PRESCRIPTION POUR UN OEIL D'UNE PERSONNE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

- **PELOUX, Marius**
94220 Charenton-le-Pont (FR)
- **BOUTINON, Stéphane**
94220 Charenton-le-Pont (FR)

(43) Date of publication of application:
28.04.2021 Bulletin 2021/17

(74) Representative: **Cabinet Novitech**
188 Grande rue Charles de Gaulle
94130 Nogent-sur-Marne (FR)

(73) Proprietor: **Essilor International**
94220 Charenton-le-Pont (FR)

(56) References cited:
WO-A1-2012/177544 **WO-A1-2019/099952**
US-A1- 2013 083 185 **US-A1- 2016 120 402**
US-A1- 2017 150 882

(72) Inventors:
• **DE ROSSI, Hélène**
94220 Charenton-le-Pont (FR)

EP 3 811 849 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

DescriptionFIELD OF THE INVENTION

[0001] The invention relates to a method and a system for determining a prescription for an eye of a wearer. The invention further relates to corresponding computer program product and computer readable medium. The invention further relates to a method for providing an ophthalmic lens adapted to a prescription of the wearer.

BACKGROUND OF THE INVENTION

[0002] WO 2019/099952 A1 discloses computer-implemented methods, apparatuses, systems, and non-transitory computer-readable storage media that enable a Rapid Deductive Refraction (RDR) stepwise eye exam to be conducted on a subject's eye with a mobile computing device. WO 2012/177544 A1 relates to an adapter system which connects an image capture device to an ophthalmoscope at multiple locations with one connection being proximate to the aligned optical axes of the image capture device and the ophthalmoscope and the other connection being distal to the aligned optical axes. US 2017/150882 A1 relates to devices, systems and computer program products for determining eye refraction.

[0003] An optical lens is generally determined to be then manufactured in accordance with the wearer specifications. In the case, for example, of an ophthalmic lens for the correction or improvement of eyesight, the ophthalmic lens is determined according to a wearer prescription corresponding to the visual requirements of that wearer.

[0004] The prescription of an eye of a person can be determined by measuring the refraction of the eye also called photorefractometry or photoretinoscopy. The principle of photorefractometry involves projecting light into the eye during flash photography and then examining the paths of light that emerge from the pupil after scattering on the back portion of the interior of the eyeball.

[0005] For example for a myopic wearer, light coming from a light source and reflected on the retina enters a camera in such a way that the camera sees a "crescent" inside the pupil of the person. The size, position and shape of this crescent depend on the refraction of the wearer's eye. For given distance between the light source and the edge of the camera aperture, also called eccentricity, working distance, camera lens diameter and pupil diameter, the size of the crescent is proportional to the refractive error. Consequently, a power, astigmatism and axis can be determined based on measurements of the refractive error in at least three different meridians defined by the axis crossing the center of the camera and the light source (Cf. "Two-dimensional simulation of eccentric photorefractometry images for ametropes: factors influencing the measurement", Y. Wu, L.N. Thibos & T.R. Candy, Ophthalmic Physiol. Opt. 2018; 38: 432-446).

[0006] Today's optometrists use accurate but cumbersome devices which require a rather long and not practical measurement to evaluate the prescription of a wearer.

5 **[0007]** Particularly in developing countries, optometrists are likely to be rare and rather low-skilled, and may not be able to afford expensive prescription measurement needs.

10 **[0008]** One object of the present invention is to provide a cheap, simple and very quick prescription measurement method and system.

SUMMARY OF THE INVENTION

15 **[0009]** To this end, the invention proposes a system for determining a prescription for an eye of a person, the system being configured to communicate with a mobile device, comprising:

- 20 - at least one first light source adapted to illuminate the eye with first light having a first optical wavelength;
- at least one second light source adapted to illuminate the eye with second light having a second optical wavelength different from the first wavelength; and
- 25 - a calculation module comprising a memory and a processor arranged to execute a program instructions stored in the memory to:

30 o measure the photorefractometry of the eye at the first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light;

35 o measure the photorefractometry of the eye at the second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light;

40 o determine the prescription for the eye based on the measured photorefractometry at the first wavelength and the measured photorefractometry at the second wavelength.

45 **[0010]** Advantageously, such system allows non-invasive, easy-to-use, cheap tool to perform digital refraction measurements, particularly in developing countries. In the sense of the invention, digital refraction measurement is refraction measurement using digital means.

50 **[0011]** Indeed, while certain range of wavelength, also called "dark zone", of a light source flashing on the eye may cause no crescent for corresponding certain refractive error, the system allows the simultaneous objective measurement of the refraction of an eye of a person at two wavelengths and consequently its prescription. Consequently, there is always a possible measurement of the refraction since at least one picture under one of both light sources should show the crescent.

55 **[0012]** In addition, the system can be advantageously removably fastened to and associated with a mobile de-

vice like a smartphone.

[0013] According to further embodiments which can be considered alone or in combination:

- the calculation module is embedded into the mobile device;
- the system for determining a prescription is further configured to be in communication with a distant unit comprising a memory and a processor arranged to execute a program instructions stored in the memory to store data relative at least to the measured photorefracton of the eye at the first wavelength, the measured photorefracton of the eye at the second wavelength;
- the system is fastened to a housing of the mobile device and removable;
- the or each first light source is configured to emit infrared or near infrared light and the or each second light source is configured to emit visible light;
- the system is configured to be in communication with a camera adapted and configured to record at least one picture of the eye of the person when the eye is illuminated by first light or second light;
- the camera is embedded into the mobile device;
- the camera is embedded into the system;
- the second light source is arranged at the same distance from the camera than the first light source;
- the system for determining the prescription of the eye comprises at least one set of three first light sources, each adapted to emit first light at the first optical wavelength;
- the first light sources of each set are equidistant from the camera and are arranged so as to define three directions regularly spaced angularly;
- the processor is arranged to execute a program instructions stored in the memory to:
 - illuminate the eye with first light emitted successively by the or each first light source emitting at the first wavelength,
 - illuminate the eye with second light by the second light source emitting at the second wavelength,
 - recording at least one picture of the eye of the person by the camera when the eye is illuminated by first light and/or second light;
- the system comprises a plurality of sets of three first light sources, the distance between the camera and the first light sources of a set is different from one set to another, the first light sources of the plurality of the sets are arranged so as to define the same three directions regularly spaced angularly, and wherein the processor is arranged to execute a program instructions stored in the memory to measure the photorefracton of the eye at the first wavelength by illuminating the eye with first light emitted successively by each first light source of at least one set of

the plurality of sets before measuring the photorefracton of the eye at the second wavelength by illuminating the eye with second light emitted by the second light source;

- the system comprises a plurality of second light sources adapted to emit light having the second optical wavelength; each second light source being equidistant from the camera and associated to one different direction define by a first light source and the camera, and wherein the processor is arranged to execute a program instructions stored in the memory to select one of the second light sources to illuminate the eye before the measurement of the photorefracton of the eye at the second wavelength based on the measurement of the photorefracton of the eye at the first wavelength;
- the system comprises a plurality of second light sources adapted to emit light having the second optical wavelength; each second light source being at different distance from the camera and associated to the same direction define by a first light source and the camera, and wherein the processor is arranged to execute a program instructions stored in the memory to select one of the second light sources to illuminate the eye before the measurement of the photorefracton of the eye at the second wavelength based on the measurement of the photorefracton of the eye at the first wavelength.

[0014] Another object of the invention is directed to a method for determining a prescription for an eye of a person with a system according to the invention, the method comprising at least:

- measuring the photorefracton of the eye at the first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light emitted successively by the or each first light source;
- measuring the photorefracton of the eye at the second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light emitted by the second light source; and
- determining the prescription for the eye based on the measured photorefracton at the first wavelength and the measured photorefracton at the second wavelength.

[0015] According to further embodiments of the method which can be considered alone or in combination:

- measuring the photorefracton of the eye at the second wavelength and measuring the photorefracton of the eye at the first wavelength are spaced temporally by less than 0.5s;
- the method further comprises determining the distance between the eye of the person and the camera;
- the method further comprises determining the inter-pupillary distance (IPD) of the person;

- the method further comprises determining the orientation of the system in relation to the eyes of the person;
- measurements are made preferably in a dark environment.

[0016] The invention further relates to a method for providing an ophthalmic lens adapted to a prescription of the wearer, the method comprising:

- determining a prescription for an eye of the wearer according to the previous method of the invention; and
- manufacturing the ophthalmic lens according to the determined prescription adapted to the eye of the wearer.

[0017] According to a further aspect, the invention further relates to a computer program product comprising one or more stored sequence of instructions that are accessible to a processor and which, when executed by the processor, causes the processor to carry out the steps of the method for determining a prescription for an eye of the wearer according to the invention, and more particularly at least the steps of:

- measuring a photorefracton of an eye at a first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light emitted by the or each first light source ;
- measuring a photorefracton of the eye at a second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light emitted by a second light source;
- determining a prescription for the eye based on the measured photorefracton at the first wavelength and the measured photorefracton at the second wavelength.

[0018] The invention also relates to a computer-readable storage medium having a program recorded thereon; where the program makes the computer execute at least the method of the invention.

[0019] The invention also relates to a computer readable medium carrying one or more sequences of instructions of the computer program product according to the invention.

[0020] Unless specifically stated otherwise, as apparent from the following discussions, it is appreciated that throughout the specification discussions utilizing terms such as "computing", "calculating", or the like, refer to the action and/or processes of a computer or computing system, or similar electronic computing device, that manipulate and/or transform data represented as physical, such as electronic, quantities within the computing system's registers and/or memories into other data similarly represented as physical quantities within the computing system's memories, registers or other such information

storage, transmission or display devices.

[0021] Embodiments of the present invention may include apparatuses for performing the operations herein. This apparatus may be specially constructed for the desired purposes, or it may comprise a general purpose computer or Digital Signal Processor ("DSP") selectively activated or reconfigured by a computer program stored in the computer. Such a computer program may be stored in a computer readable storage medium, such as, but is not limited to, any type of disk including floppy disks, optical disks, CD-ROMs, magnetic-optical disks, read-only memories (ROMs), random access memories (RAMs) electrically programmable read-only memories (EPROMs), electrically erasable and programmable read only memories (EEPROMs), magnetic or optical cards, or any other type of media suitable for storing electronic instructions, and capable of being coupled to a computer system bus.

[0022] The processes and displays presented herein are not inherently related to any particular computer or other apparatus. Various general purpose systems may be used with programs in accordance with the teachings herein, or it may prove convenient to construct a more specialized apparatus to perform the desired method.

[0023] The desired structure for a variety of these systems will appear from the description below. In addition, embodiments of the present invention are not described with reference to any particular programming language. It will be appreciated that a variety of programming languages may be used to implement the teachings of the inventions as described herein.

BRIEF DESCRIPTION OF THE DRAWINGS

[0024] Embodiments of the invention will now be described, by way of example only, and with reference to the following drawings in which:

- Figures 1 and 2 is a perspective view of a system for determining the prescription of an eye of a person according to the invention;
- Figure 3 is a schematic diagram of a system adapted to determine the prescription of an eye of a person according to a first embodiment of the invention;
- Figure 4 is an illustration of a chart-flow of a method for determining a prescription of an eye of a person according to the first embodiment of the invention;
- Figure 5 shows an illustration of a light sources arrangement which can be used in a system for determining the prescription of an eye according to a second embodiment of the invention;
- Figure 6 is an illustration of a chart-flow of a method for determining a prescription of an eye of a person according to the second embodiment of the invention;
- Figure 7 shows an illustration of a light sources arrangement which can be used in a system for determining the prescription of an eye according to a third

- embodiment of the invention;
- Figure 8 is an illustration of a chart-flow of a method for determining a prescription of an eye of a person according to the third and a fourth embodiments of the invention; and
- Figure 9 shows an illustration of a light sources arrangement which can be used in a system for determining the prescription of an eye according to a fourth embodiment of the invention.

[0025] Elements in the figures are illustrated for simplicity and clarity and have not necessarily been drawn to scale. For example, the dimensions of some of the elements in the figure may be exaggerated relative to other elements to help improve the understanding of the embodiments of the present invention.

DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

[0026] The invention relates to a method and a system for determining a prescription for an eye of a person. Such system is adapted and configured to implement the method for determining a prescription for an eye of a person according to the invention.

[0027] The prescription comprises a set of optical characteristics such as spherical power, cylindrical power, cylinder axis, addition power, and prescribed prism, determined by an ophthalmologist in order to correct the vision defects of the wearer.

[0028] With reference to figures 1 and 2, the system 10 according to the invention is configured to communicate with a mobile device 12, in particular a smartphone. For example, the system 10 can communicate with or via the mobile device 12 in a wired or wireless manner.

[0029] Preferably, the system is adapted to be fastened to a housing 14 of the mobile device 12 as illustrated on figures 1 and 2.

[0030] The system 10 is illustrated before being fastened to the mobile device 12 on figure 1 and after being fastened to a housing 14 of the mobile device 12 on figure 2.

[0031] In the following description, smartphones are used as examples of such mobile system. Nevertheless, other mobile systems can also be used such as tablet personal computers or laptop computers.

[0032] Figure 3 shows a schematic illustration of the system 10 according to a first embodiment of the invention.

[0033] The system 10 comprises a first light source 16 and a second light source 18. The first and second light sources 16, 18 are each adapted to illuminate an eye 2 of the person with respectively first light 20 having a first optical wavelength and second light 22 having a second optical wavelength. The second optical wavelength is different from the first optical wavelength.

[0034] Each of the first and second light sources 16, 18 may be configured to illuminate the eye directly or

indirectly, for example by being reflected by a mirror.

[0035] Preferably, the first light source is configured to emit infrared or near infrared light so as not to change the pupil diameter during a refraction measurement and thus, the prescription determining.

[0036] The second light source is preferably configured to emit visible light, for example configured to emit green light at around 550 nm. Visible light allows overcoming the drawback of the shift in the prescription determining induced by using infrared light and the fact that the eye is very chromatic.

[0037] The second light source may be configured to emit red light allowing a better reflection of the retina.

[0038] Preferably, the light sources are light-emitting diode (LED). Preferably the bandwidth of the spectrum of the light sources is very narrow, less than 50 nm at half width .

[0039] Infrared LEDs with different spectral bands could also be considered for more accurate extrapolation of a model of the prescription function of the wavelength.

[0040] The system 10 further comprises a camera 30 adapted and configured to record at least one picture of the eye of the person when the eye is illuminated by first light or second light.

[0041] A very narrow band pass filter, *i.e.* less than 50 nm at half width, could be applied to the camera so that the camera only collects infrared signal from the sources and their reflections on the retina, not from the sun or from any incandescent lamp for instance, that could affect the measurement results, when one of the used wavelength is infrared. Alternatively, the filter may also be a high-pass filter, with no light other than infrared light passing.

[0042] Preferably, the camera is embedded in the system 10 such that it can acquire picture of the eye of the person in "selfie" mode or in "standard photo" mode. The person could also take a picture of himself in front of a flat mirror to perform his/her refraction measurement.

[0043] In addition, the system could also be inclined in relation to the smartphone to meet a best ergonomic needs.

[0044] While in the preferred embodiment, the camera is embedded in the system, the camera can be embedded in the smartphone and the system is configured to be in communication with the camera of the smartphone and arranged such that the camera of the smartphone can record pictures of the eye of the person when the eye is illuminated by first light or second light.

[0045] Preferably, the second light source 18 is arranged at the same distance as the first light source 16 from the camera 30. The distance between the first light source or the second light source and the camera is preferably comprised between 0 and 30 mm.

[0046] The system further comprises a calculation module 40 comprising a memory 42 and a processor 44 arranged to execute a program instructions stored in the memory to implement the method for determining a prescription for an eye of a person according to the invention.

[0047] With reference to figure 4, the method comprises:

- a first illuminating step S10,
- a first acquisition step S12
- a first photorefractive measuring step S14,
- a second illuminating step S20,
- a second acquisition step S22
- a second photorefractive measuring step S24,
- a prescription determining step S30.

[0048] During the first illuminating step S10, the eye 2 of the person is illuminated with first light 20 having the first optical wavelength by the first light source 16.

[0049] Then, at least one first picture is acquired by the camera 30 and recorded when illuminating the eye 2 with first light 20 in S12.

[0050] During the first photorefractive measuring step S14, the photorefractive of the eye at the first wavelength is measured based on the first picture(s) of the eye recorded when illuminating the eye with first light.

[0051] Photorefractive is an objective refraction method based on a picture of light reflection by the retina. The refractive state can be calculated from the magnitude and position of this light reflection using a mathematical formula or from a physical simulation model.

[0052] During the second illuminating step S20, the same eye 2 of the person is illuminated with second light 22 having the second optical wavelength by the second light source 18.

[0053] Then, at least one second picture is acquired by the camera 30 and recorded when illuminating the eye 2 with second light in S22.

[0054] During the second photorefractive measuring step S24, the photorefractive of the eye at the second wavelength is measured based on the at least one second picture of the eye recorded when illuminating the eye with second light.

[0055] The second illuminating step should follow quickly the first illuminating step, i.e. fast enough so that the eye pupil has not time to reduce to ensure a large size of pupil and to avoid eye movements, eye blinks... Preferably, measuring the photorefractive of the eye at the second wavelength and measuring the photorefractive of the eye at the first wavelength are spaced temporally by less than 0.5s.

[0056] Then, the prescription for the eye is determined based on the measured photorefractive at the first wavelength and the measured photorefractive at the second wavelength in S30.

[0057] More particularly, the measured power at the first wavelength and the measured power at the second wavelength may be compared and used to correct the first refraction measurement of the person's eye to determine the prescription of the person's eye.

[0058] Alternatively, it is possible to mix the above individualized first and second refraction measurements with an average correction table via a weighting function.

[0059] Preferably, the calculation module 40 is embedded into the smartphone 12. Alternatively, the calculation module 40 may be embedded into the system 10. Thus, the refraction measurements and the prescription determining are performed via a local analysis within an application that applies pattern recognition algorithms for measuring the size, position and shape of the crescent, as well as the pupil diameter.

[0060] Nevertheless, the calculation module 40 may be embedded at least partly into the mobile device 10 and/or the smartphone 12 and/or a distant unit (not illustrated).

[0061] Indeed, the system 10 for determining a prescription may further be configured to be in communication with a distant unit comprising a memory and a processor arranged to execute a program instructions stored in the memory to store data relative at least to the measured photorefractive of the eye at the first wavelength, the measured photorefractive of the eye at the second wavelength. Then, the determining of the prescription of the eye S30 may also be implemented by the distant unit when the processor of the distant unit executes a corresponding program instructions stored in the memory of the distant unit. In this case, the measured data is stored in a cloud, recognition and/or machine learning algorithms are used for analyzing the results. In this case person accounts could be created to track the evolution of the prescription of a person with correlated graphics in an application.

[0062] Measurements are preferably made in a low light environment to expand the person's pupil to a maximal value, which reduces the width of the dark zone.

[0063] Furthermore, the method may advantageously comprises a step for determining the distance between the eye of the person and the camera. The distance measurement can be made thanks to a simple 1 -pixel time-of-flight (ToF) sensor or to a ToF pixel array. Nevertheless, a sensor measuring the quantity of light reflected from the measured object may also be used to determine the distance between the eye of the person and the camera.

[0064] The distance may also be determined thanks to a stereoscopic combination of images acquired from the camera of the smartphone and images acquired from the camera of the system. The distance may also be determined thanks to the front or rear camera of the Smartphone or the camera of the system and an associated image processing. For example, the distance could be estimated considering that the iris size is approximately the same for everybody. In another embodiment, the person using the system may wear some goggles whose size is well-known, as a reference to estimate the distance between the eye and one of the camera.

[0065] The method may further advantageously comprises a step for determining the interpupillary distance (IPD) of the person.

[0066] Advantageously, the method may further comprises a step for determining the orientation of the system

in relation to the eyes of the person in order to determine precisely the axis of the astigmatism. This orientation may be determined using the inertial motion unit (IMU) of the smartphone. Another way to evaluate this orientation is to evaluate the angle of the line separating the two eye centers in relation to an axe defined between a normal axis to the aperture of the camera of the system and the line separating the two eye centers.

[0067] In addition, while in the embodiment as presently described, the first photorefractive measuring step S14 is implemented before the second illuminating step S20 and the second acquisition step S22, it will be understood, that in alternative embodiments of the invention, the photorefractive measurement at the first wavelength may be implemented after all acquisitions at first and second wavelengths are performed in order to reduce the measurement time since the photorefractive measurement steps can may take some time.

[0068] Figure 5 illustrates a second and preferred embodiment of the system according to the invention. This second embodiment differs from the previous one in that the system comprises a set of three first light sources 16A, 16B and 16C, each adapted to illuminate the eye 2 of the person with respectively first light 20 having the first optical wavelength.

[0069] In this preferred embodiment, the system still has only one second light source 18.

[0070] The first light sources 16A, 16B and 16C of the set are arranged to be equidistant from the camera 30 and to define three directions regularly spaced angularly also called meridians X_A , X_B and X_C .

[0071] Furthermore, the second light source 18 is preferably arranged at the same distance than the first light source 16 from the camera 30.

[0072] According to this second embodiment, the processor 44 is arranged to execute a program instructions stored in the memory 42 to implement a second embodiment of the method for determining the prescription of the eye of the person according to the invention.

[0073] With reference to figure 6, the second embodiment of the method differs from the previous one in that the step S10 for illuminating the eye with first light and the step S12 for acquiring and recording the corresponding first pictures by the camera when the eye is illuminated with first light are repeated successively for each first light source 16A, 16B and 16C of the set. The step for illuminating the eye by the first light source 16K is denoted S10-K and the step for acquiring and recording the corresponding first pictures by the camera when the eye is illuminated by the first light source 16K is denoted S12-K, K being A, B or C. Thus, the photorefractive of the eye at the first wavelength is measured before measuring the photorefractive of the eye at the second wavelength by illuminating the eye with second light emitted by the second light source.

[0074] In other words, all the measurements at the first wavelength are done before the single measurement at the second wavelength.

[0075] Such second embodiment allows an accurate measurement of eye refraction at infrared wavelength thanks to the measurements in three directions X_A , X_B and X_C and for several distances between the set of first light sources and the camera and consequently, an accurate determining of the prescription for the eye of the person. Indeed, thanks to the measurements in three directions X_A , X_B and X_C the complete refraction may be determined, i.e. power, astigmatism and axis.

[0076] Figure 7 illustrates a third embodiment of the system according to the invention. This third embodiment differs from the previous ones in that the system comprises a plurality of sets n of three first light sources 16-A_{*i*}, 16-B_{*i*} and 16-C_{*i*} for i an integer between 1 and n . Each first light source is adapted to illuminate the eye 2 of the person with respectively first light 20 having the first optical wavelength.

[0077] For each set i , the first light sources 16-A_{*i*}, 16-B_{*i*} and 16-C_{*i*} are arranged to be equidistant from the camera 30. Of course, the distance between the camera and the first light sources of a set is different from one set to another. The first light sources of the sets are arranged on the three meridians X_A , X_B and X_C .

[0078] In this third embodiment, the system comprises a plurality of second light sources adapted to emit light having the second optical wavelength, preferably three second light sources 18-A, 18-B, 18-C as illustrated on figure 7.

[0079] The three second light sources 18-A, 18-B, 18-C are equidistant from the camera and are preferably regularly angularly spaced.

[0080] The three second light sources 18-A, 18-B, 18-C are arranged at the same distance from the camera than a set of three first light sources.

[0081] Each second light source 18-A, 18-B, 18-C is associated to one different meridian X_A , X_B and X_C .

[0082] According to this third embodiment, all the measurements at the first wavelength are done before the single measurement at the second wavelength. Thus, the processor 44 is arranged to execute a program instructions stored in the memory to measure the photorefractive of the eye at the first wavelength by illuminating the eye with first light emitted successively by each first light source of at least one set of the plurality of sets before measuring the photorefractive of the eye at the second wavelength by illuminating the eye with second light emitted by the second light source.

[0083] Advantageously, the processor may be further arranged to execute a program instructions stored in the memory to implement a step S40 for selecting one of the second light sources to illuminate the eye before the measurement of the photorefractive of the eye at the second wavelength based on the measurement of the photorefractive of the eye at the first wavelength. Indeed, a first estimate of the eye refraction can be obtained from the first photorefractive measuring step S14 allowing to define a strategy for selecting the visible source to switch on. For example, the second light source associated to

the meridian for which the infrared measurement is the most precise may be selected to have best accuracy for visible measurement.

[0084] Such third embodiment allows an accurate measurement of eye refraction at infrared wavelength thanks to the measurements in three directions X_A , X_B and X_C and for several distances between the set of first light sources and the camera and consequently, an accurate determining of the prescription for the eye of the person. Indeed, thanks to the measurements in three directions X_A , X_B and X_C the complete refraction may be determined, i.e. power, astigmatism and axis.

[0085] In addition, the use of several sets of first light sources at different distances from the camera allows a more precise first refraction measurement and thus a more accurate determination of the prescription especially when this one is important.

[0086] Figure 9 shows a fourth embodiment of the system according to the invention compatible with the previous one. This fourth embodiment differs from the third embodiment in that the system comprises a plurality of second light sources 18-i adapted to emit light having the second optical wavelength and arranged in another way which will be detailed hereinafter.

[0087] Three second light sources 18-1, 18-2, 18-3 are illustrated on figure 9.

[0088] Each second light source 18-i is associated to a set i of three first light sources 16-A $_i$, 16-B $_i$, 16-C $_i$ and is thus arranged at the same distance from the camera 30 than all the three first light sources of the set i . Thus, each second light source 18-1, 18-2, 18-3 is arranged at different distance from the camera 30.

[0089] According to this fourth embodiment, with reference to the flow chart in figure 8, the processor may be advantageously further arranged to execute a program instructions stored in the memory to implement a step S40 for selecting one of the second light sources to illuminate the eye before the measurement of the photorefractive of the eye at the second wavelength based on the measurement of the photorefractive of the eye at the first wavelength. Indeed, a first estimate of the eye refraction can be obtained from the first photorefractive measuring step S14 allowing to define a strategy for selecting the visible source to switch on. For example, the second light source arranged at a distance from the camera providing a measurement for which the eye refraction is not in the dark zone, based on the first refraction measurement may be selected to have best accuracy for visible measurement, and taking into account the intrinsic chromatism of the eye between first light and second light and more particularly in the case of infrared light and visible light.

[0090] Such fourth embodiment allows an accurate measurement of eye refraction at infrared wavelength thanks to the measurements in three directions X_A , X_B and X_C and for several distances between the set of first light sources and the camera and consequently, an accurate determining of the prescription for the eye of the

person. Indeed, thanks to the measurements in three directions X_A , X_B and X_C the complete refraction may be determined, i.e. power, astigmatism and axis.

[0091] In addition, the use of several sets of first and second light sources at different distances from the camera allows more precise refraction measurements and thus a more accurate determination of the prescription especially when this one is important.

[0092] Another object of the invention is a method for providing an ophthalmic lens adapted to a prescription of the wearer, the method comprising:

- determining a prescription for an eye of the wearer according to the invention and as previously described; and
- manufacturing the ophthalmic lens according to the determined prescription adapted to the eye of the wearer.

[0093] The invention as disclosed hereinbefore has the advantage to provide a non-invasive, easy-to-use, cheap tool to perform e-refraction measurements, particularly in developing countries.

[0094] Indeed, the combination of measurements at two wavelengths and more particularly with an infrared light source to get large pupil and with a visible light source allows an accurate determination of the prescription for an eye of a person.

[0095] In addition, the invention can be easily performed on children and thus can provide a simple system for parents that want to monitor the evolution of the prescription of their children.

[0096] Furthermore, the invention allows measuring accurately the interpupillary distance of a person which is a very important parameter to provide to a wearer an appropriate pair of eyeglasses.

[0097] The invention has been described above with the aid of embodiments without limitation of the general inventive concept.

[0098] Many further modifications and variations will suggest themselves to those skilled in the art upon making reference to the foregoing illustrative embodiments, which are given by way of example only and which are not intended to limit the scope of the invention, that being determined solely by the appended claims.

[0099] Indeed, while in the disclosed embodiments, the acquisitions corresponding to each light source is performed sequentially, some of the acquisitions could be performed simultaneously to decrease the measurement time.

[0100] Alternatively, the first light sources may be infrared sources and the second light sources may be configured to emit blue light at around 550 nm. In this case, a weighted average of the measured refraction with both wavelengths corresponds to the real refraction and thus to the good prescription.

[0101] According to another embodiment, the system may comprise waveguides associated to some of the first

and/or second light sources, for instance the most central light sources, so as to fictitiously bring the light sources closer to the camera.

[0102] In the claims, the word "comprising" does not exclude other elements or steps, and the indefinite article "a" or "an" does not exclude a plurality. The mere fact that different features are recited in mutually different dependent claims does not indicate that a combination of these features cannot be advantageously used.

Claims

1. System (10) for determining a prescription for an eye (2) of a person, the system being configured to communicate with a mobile device (12), comprising:
 - at least one first light source (16) adapted to illuminate the eye with first light (20) having a first optical wavelength;
 - at least one second light source (18) adapted to illuminate the eye with second light (22) having a second optical wavelength different from the first wavelength; and
 - a calculation module (40) comprising a memory (42) and a processor (44) arranged to execute a program instructions stored in the memory to:
 - o measure the photorefractive of the eye (2) at the first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light (20);
 - o measure the photorefractive of the eye (2) at the second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light (22);
 - o determine the prescription for the eye (2) based on the measured photorefractive at the first wavelength and the measured photorefractive at the second wavelength.
2. The system according to claim 1, wherein the calculation module (40) is embedded into the mobile device (12).
3. The system according to claim 1 or 2, wherein the system (10) for determining a prescription is further configured to be in communication with a distant unit comprising a memory and a processor arranged to execute a program instructions stored in the memory to store data relative at least to the measured photorefractive of the eye at the first wavelength, the measured photorefractive of the eye at the second wavelength.
4. The system according to any of claims 1 to 3, wherein the system (10) is configured to be removably fastened to a housing (14) of the mobile device (12).
5. The system according to any of claims 1 to 4, wherein the or each first light source (16) is configured to emit infrared or near infrared light and the or each second light source (18) is configured to emit visible light.
6. The system according to any of claims 1 to 5, wherein the second light source (18) is arranged at the same distance than the first light source (16) from a camera (30) adapted and configured to record at least one picture of the eye (2) of the person when the eye is illuminated by first light (20) or second light (22).
7. The system according to any of claims 1 to 6, wherein the system (10) for determining the prescription of the eye comprises at least one set of three first light sources (16A, 16B, 16C), each adapted to emit first light at the first optical wavelength.
8. The system according to claim 7, wherein the first light sources (16A, 16B, 16C) of each set are equidistant from a camera (30) adapted and configured to record at least one picture of the eye (2) of the person when the eye is illuminated by first light (20) or second light (22) and are arranged so as to define three directions (X_A , X_B , X_C) regularly spaced angularly.
9. The system according to any of claims 1 to 8, wherein the processor (44) is arranged to execute a program instructions stored in the memory (42) to:
 - illuminate the eye (2) with first light (20) emitted successively by the or each first light source (16) emitting at the first wavelength,
 - illuminate the eye (2) with second light (22) by the second light source (18) emitting at the second wavelength,
 - recording at least one picture of the eye of the person by a camera (30) adapted and configured to record at least one picture of the eye of the person when the eye is illuminated by first light (20) or second light (22).
10. The system according to any of claims 7 to 9, wherein the system (10) comprises a plurality of sets of three first light sources (16-Ai, 16-Bi, 16-Ci), the distance between the camera (30) and the first light sources of a set is different from one set to another, the first light sources of the plurality of the sets are arranged so as to define the same three directions (X_A , X_B , X_C) regularly spaced angularly, and wherein the processor (44) is arranged to execute a program instructions stored in the memory to measure the photorefractive of the eye at the first wavelength by illuminating the eye with first light emitted successively by each first light source of at least one set of the plurality of sets before measuring the photorefractive of the eye at the second wavelength by

illuminating the eye with second light emitted by the second light source.

11. Method for determining a prescription for an eye of a person with a system (10) for determining a prescription for an eye (2) of a person, the system being configured to communicate with a mobile device (12), comprising:

- at least one first light source (16) adapted to illuminate the eye with first light (20) having a first optical wavelength;
- at least one second light source (18) adapted to illuminate the eye with second light (22) having a second optical wavelength different from the first wavelength; and
- a calculation module (40) comprising a memory (42) and a processor (44) arranged to execute a program instructions stored in the memory to:

- o measure the photorefractive of the eye (2) at the first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light (20);

- o measure the photorefractive of the eye (2) at the second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light (22);

- o determine the prescription for the eye (2) based on the measured photorefractive at the first wavelength and the measured photorefractive at the second wavelength.,

the method comprising at least:

- measuring the photorefractive of the eye at the first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light emitted successively by the or each first light source (16);
- measuring the photorefractive of the eye at the second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light emitted by the second light source (18); and
- determining the prescription for the eye based on the measured photorefractive at the first wavelength and the measured photorefractive at the second wavelength.

12. The method according to claim 11 further comprises determining the distance between the eye (2) of the person and the camera (30).

13. Method for providing an ophthalmic lens adapted to a prescription of the wearer, the method comprising:

- determining a prescription for an eye of the

wearer according to any of the preceding claims 11 or 12; and

- manufacturing the ophthalmic lens according to the determined prescription adapted to the eye of the wearer.

14. A computer program product comprising one or more stored sequences of instructions that are accessible to a processor and which, when executed by the processor, causes the processor to carry out at least the steps of:

- measuring a photorefractive of an eye at a first wavelength based on at least one picture of the eye recorded when illuminating the eye with first light emitted by the or each first light source ;

- measuring a photorefractive of the eye at a second wavelength based on at least one picture of the eye recorded when illuminating the eye with second light emitted by a second light source;

- determining a prescription for the eye based on the measured photorefractive at the first wavelength and the measured photorefractive at the second wavelength.

15. A computer readable medium carrying out one or more sequences of instructions of the computer program product of claim 14.

Patentansprüche

1. System (10) zum Bestimmen eines Rezepts für ein Auge (2) einer Person, wobei das System konfiguriert ist, um mit einem Mobilgerät (12) zu kommunizieren, umfassend:

- mindestens eine erste Lichtquelle (16), die ausgelegt ist, um das Auge mit erstem Licht (20) mit einer ersten optischen Wellenlänge zu beleuchten;

- mindestens eine zweite Lichtquelle (18), die ausgelegt ist, um das Auge mit zweitem Licht (22) mit einer zweiten optischen Wellenlänge zu beleuchten, die sich von der ersten Wellenlänge unterscheidet; und

- ein Berechnungsmodul (40), umfassend einen Speicher (42) und einen Prozessor (44), der angeordnet ist, um in dem Speicher gespeicherte Programmanweisungen auszuführen, zum:

- o Messen der Photorefraktion des Auges (2) an der ersten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit erstem Licht (20) aufgezeichnet wurde;

- o Messen der Photorefraktion des Auges

- (2) an der zweiten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit zweitem Licht (22) aufgezeichnet wurde;
 o Bestimmen des Rezepts für das Auge (2) basierend auf der gemessenen Photorefraktion bei der ersten Wellenlänge und der gemessenen Photorefraktion bei der zweiten Wellenlänge.
2. System nach Anspruch 1, wobei das Berechnungsmodul (40) in das Mobilgerät (12) eingebettet ist.
 3. System nach Anspruch 1 oder 2, wobei das System (10) zum Bestimmen eines Rezepts ferner konfiguriert ist, um in Kommunikation mit einer entfernten Einheit zu sein, die einen Speicher und einen Prozessor umfasst, der zum Ausführen von Programmanweisungen angeordnet ist, die in dem Speicher gespeichert sind, um Daten zu speichern, die mindestens die gemessene Photorefraktion des Auges bei der ersten Wellenlänge und die gemessene Photorefraktion des Auges bei der zweiten Wellenlänge betreffen.
 4. System nach einem der Ansprüche 1 bis 3, wobei das System (10) konfiguriert ist, um abnehmbar an einem Gehäuse (14) des Mobilgeräts (12) befestigt zu sein.
 5. System nach einem der Ansprüche 1 bis 4, wobei die oder jede erste Lichtquelle (16) ausgestaltet ist, um Infrarot- oder nahes Infrarotlicht zu emittieren, und die oder jede zweite Lichtquelle (18) konfiguriert ist, um sichtbares Licht zu emittieren.
 6. System nach einem der Ansprüche 1 bis 5, wobei die zweite Lichtquelle (18) in dem gleichen Abstand wie die erste Lichtquelle (16) von einer Kamera (30) angeordnet ist, die ausgelegt und konfiguriert ist, um mindestens ein Bild des Auges (2) der Person aufzuzeichnen, wenn das Auge durch erstes Licht (20) oder zweites Licht (22) beleuchtet wird.
 7. System nach einem der Ansprüche 1 bis 6, wobei das System (10) zum Bestimmen des Rezepts des Auges mindestens einen Satz von drei ersten Lichtquellen (16A, 16B, 16C) umfasst, wovon jede ausgelegt ist, um erstes Licht mit der ersten optischen Wellenlänge zu emittieren.
 8. System nach Anspruch 7, wobei die ersten Lichtquellen (16A, 16B, 16C) jedes Satzes äquidistant zu einer Kamera (30) sind, die ausgelegt und konfiguriert ist, um mindestens ein Bild des Auges (2) der Person aufzuzeichnen, wenn das Auge durch erstes Licht (20) oder zweites Licht (22) beleuchtet wird, und so angeordnet sind, dass drei Richtungen (XA, XB, XC) definiert werden, die regelmäßig im Winkel beabstandet sind.
 9. System nach einem der Ansprüche 1 bis 8, wobei der Prozessor (44) angeordnet ist, um in dem Speicher (42) gespeicherte Programmanweisungen auszuführen, zum:
 - Beleuchten des Auges (2) mit erstem Licht (20) das nacheinander durch die oder jede erste Lichtquelle (16) emittiert wird, die mit der ersten Wellenlänge emittiert,
 - Beleuchten des Auges (2) mit zweitem Licht (22) durch die zweite Lichtquelle (18), die mit der ersten Wellenlänge emittiert,
 - Aufzeichnen von mindestens einem Bild des Auges der Person durch eine Kamera (30), die ausgelegt und konfiguriert ist, um mindestens ein Bild des Auges der Person aufzuzeichnen, wenn das Auge durch erstes Licht (20) oder zweites Licht (22) beleuchtet wird.
 10. System nach einem der Ansprüche 7 bis 9, wobei das System (10) eine Vielzahl von Sätzen von drei ersten Lichtquellen (16-Ai, 16-Bi, 16-Ci) umfasst, der Abstand zwischen der Kamera (30) und den ersten Lichtquellen eines Satzes sich von einem Satz zu einem anderen unterscheidet, die ersten Lichtquellen der Vielzahl der Sätze so angeordnet sind, dass dieselben drei Richtungen (XA, XB, XC) regelmäßig im Winkel beabstandet definiert sind, und wobei der Prozessor (44) so angeordnet ist, dass Programmanweisungen, die im Speicher gespeichert sind, ausgeführt werden, um die Photorefraktion des Auges bei der ersten Wellenlänge zu messen, indem das Auge mit erstem Licht beleuchtet wird, das nacheinander durch jede erste Lichtquelle von mindestens einem Satz der Vielzahl von Sätzen emittiert wird, bevor die Photorefraktion des Auges bei der zweiten Wellenlänge gemessen wird, indem das Auge mit zweitem Licht beleuchtet wird, das durch die zweite Lichtquelle emittiert wird.
 11. Verfahren zum Bestimmen eines Rezepts für ein Auge einer Person mit einem System (10) zum Bestimmen eines Rezepts für ein Auge (2) einer Person, wobei das System konfiguriert ist, um mit einem Mobilgerät (12) zu kommunizieren, umfassend:
 - mindestens eine erste Lichtquelle (16), die ausgelegt ist, um das Auge mit erstem Licht (20) mit einer ersten optischen Wellenlänge zu beleuchten;
 - mindestens eine zweite Lichtquelle (18), die ausgelegt ist, um das Auge mit zweitem Licht (22) mit einer zweiten optischen Wellenlänge zu beleuchten, die sich von der ersten Wellenlänge unterscheidet; und

- ein Berechnungsmodul (40), umfassend einen Speicher (42) und einen Prozessor (44), der angeordnet ist, um in dem Speicher gespeicherte Programmanweisungen auszuführen, zum:

- o Messen der Photorefraktion des Auges (2) an der ersten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit erstem Licht (20) aufgezeichnet wurde;
- o Messen der Photorefraktion des Auges (2) an der zweiten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit zweitem Licht (22) aufgezeichnet wurde;
- o Bestimmen des Rezepts für das Auge (2) basierend auf der gemessenen Photorefraktion bei der ersten Wellenlänge und der gemessenen Photorefraktion bei der zweiten Wellenlänge,

wobei das Verfahren mindestens umfasst:

- Messen der Photorefraktion des Auges bei der ersten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit erstem Licht aufgezeichnet wurde, das nacheinander durch die oder jede erste Lichtquelle (16) emittiert wird;
- Messen der Photorefraktion des Auges bei der zweiten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit zweitem Licht aufgezeichnet wurde, das durch die zweite Lichtquelle (18) emittiert wird; und
- Bestimmen des Rezepts für das Auge basierend auf der gemessenen Photorefraktion an der ersten Wellenlänge und der gemessenen Photorefraktion an der zweiten Wellenlänge.

12. Verfahren nach Anspruch 11, das des Weiteren Bestimmen des Abstands zwischen dem Auge (2) der Person und der Kamera (30) umfasst.

13. Verfahren zum Bereitstellen einer ophthalmischen Linse, die für ein Rezept des Trägers ausgelegt ist, wobei das Verfahren umfasst:

- Bestimmen eines Rezepts für ein Auge des Trägers gemäß einem der vorhergehenden Ansprüche 11 oder 12; und
- Fertigen der ophthalmischen Linse gemäß dem bestimmten Rezept, das für das Auge des Trägers ausgelegt ist.

14. Computerprogrammprodukt, umfassend eine oder mehrere gespeicherte Sequenzen von Anweisungen, die für einen Prozessor zugänglich sind, und

die bei Ausführung durch den Prozessor bewirken, dass der Prozessor mindestens die folgenden Schritte durchführt:

- 5 - Messen einer Photorefraktion eines Auges bei einer ersten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit erstem Licht aufgezeichnet wurde, das nacheinander durch die oder jede erste Lichtquelle emittiert wird;
- 10 - Messen einer Photorefraktion des Auges bei einer zweiten Wellenlänge basierend auf mindestens einem Bild des Auges, das beim Beleuchten des Auges mit zweitem Licht aufgezeichnet wurde, das durch die zweite Lichtquelle emittiert wird;
- 15 - Bestimmen eines Rezepts für das Auge basierend auf der gemessenen Photorefraktion bei der ersten Wellenlänge und der gemessenen Photorefraktion bei der zweiten Wellenlänge.

15. Computerlesbares Medium, das eine oder mehrere Sequenzen von Anweisungen des Computerprogrammprodukts gemäß Anspruch 14 ausführt.

Revendications

1. Système (10) de détermination d'une prescription pour un œil (2) d'une personne, le système étant configuré pour communiquer avec un dispositif mobile (12), comprenant :

- au moins une première source de lumière (16) adaptée pour éclairer l'œil avec une première lumière (20) ayant une première longueur d'onde optique ;
- au moins une deuxième source de lumière (18) adaptée pour éclairer l'œil avec une deuxième lumière (22) ayant une deuxième longueur d'onde optique différente de la première longueur d'onde ; et
- un module de calcul (40) comprenant une mémoire (42) et un processeur (44) agencé pour exécuter un programme d'instructions stocké dans la mémoire pour :

- mesurer la photoréfraction de l'œil (2) à la première longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec la première lumière (20) ;
- mesurer la photoréfraction de l'œil (2) à la deuxième longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec la deuxième lumière (22) ;
- déterminer la prescription pour l'œil (2) sur

- la base de la photoréfraction mesurée à la première longueur d'onde et de la photoréfraction mesurée à la deuxième longueur d'onde.
2. Système selon la revendication 1, le module de calcul (40) étant intégré dans le dispositif mobile (12).
 3. Système selon la revendication 1 ou 2, le système (10) pour déterminer une prescription étant en outre configuré pour être en communication avec une unité distante comprenant une mémoire et un processeur agencé pour exécuter un programme d'instructions stocké dans la mémoire pour stocker des données relatives au moins à la photoréfraction mesurée de l'œil à la première longueur d'onde, à la photoréfraction mesurée de l'œil à la deuxième longueur d'onde.
 4. Système selon l'une quelconque des revendications 1 à 3, le système (10) étant configuré pour être fixé de manière amovible à un boîtier (14) du dispositif mobile (12).
 5. Système selon l'une quelconque des revendications 1 à 4, la ou chaque première source de lumière (16) étant configurée pour émettre une lumière infrarouge ou proche de l'infrarouge et la ou chaque deuxième source de lumière (18) étant configurée pour émettre une lumière visible.
 6. Système selon l'une quelconque des revendications 1 à 5, la deuxième source de lumière (18) étant agencée à la même distance que la première source de lumière (16) d'une caméra (30) adaptée et configurée pour enregistrer au moins une image de l'œil (2) de la personne lorsque l'œil est éclairé par la première lumière (20) ou la deuxième lumière (22).
 7. Système selon l'une quelconque des revendications 1 à 6, le système (10) de détermination de la prescription de l'œil comprenant au moins un ensemble de trois premières sources de lumière (16A, 16B, 16C), chacune adaptée pour émettre une première lumière à la première longueur d'onde optique.
 8. Système selon la revendication 7, les premières sources de lumière (16A, 16B, 16C) de chaque ensemble étant équidistantes d'une caméra (30) adaptée et configurée pour enregistrer au moins une image de l'œil (2) de la personne lorsque l'œil est éclairé par la première lumière (20) ou la deuxième lumière (22) et étant agencées de manière à définir trois directions (X_A , X_B , X_C) régulièrement espacées angulairement.
 9. Système selon l'une quelconque des revendications 1 à 8, le processeur (44) étant agencé pour exécuter un programme d'instructions stocké dans la mémoire (42) pour :
 - éclairer l'œil (2) avec une première lumière (20) émise successivement par la ou chaque première source de lumière (16) émettant à la première longueur d'onde,
 - éclairer l'œil (2) avec une deuxième lumière (22) émise par la deuxième source de lumière (18) émettant à la deuxième longueur d'onde,
 - enregistrer au moins une image de l'œil de la personne au moyen d'une caméra (30) adaptée et configurée pour enregistrer au moins une image de l'œil de la personne lorsque l'œil est éclairé par la première lumière (20) ou la deuxième lumière (22).
 10. Système selon l'une quelconque des revendications 7 à 9, le système (10) comprenant une pluralité d'ensembles de trois premières sources de lumière (16-Ai, 16-Bi, 16-Ci), la distance entre la caméra (30) et les premières sources de lumière d'un ensemble étant différente d'un ensemble à l'autre, les premières sources de lumière de la pluralité des ensembles étant agencées de manière à définir les mêmes trois directions (X_A , X_B , X_C) régulièrement espacées angulairement, et le processeur (44) étant agencé pour exécuter un programme d'instructions stocké dans la mémoire afin de mesurer la photoréfraction de l'œil à la première longueur d'onde en éclairant l'œil avec la première lumière émise successivement par chaque première source de lumière d'au moins un ensemble de la pluralité d'ensembles avant de mesurer la photoréfraction de l'œil à la deuxième longueur d'onde en éclairant l'œil avec la deuxième lumière émise par la deuxième source de lumière.
 11. Procédé de détermination d'une prescription pour un œil d'une personne avec un système (10) de détermination d'une prescription pour un œil (2) d'une personne, le système étant configuré pour communiquer avec un dispositif mobile (12), comprenant :
 - au moins une première source de lumière (16) adaptée pour éclairer l'œil avec une première lumière (20) ayant une première longueur d'onde optique ;
 - au moins une deuxième source de lumière (18) adaptée pour éclairer l'œil avec une deuxième lumière (22) ayant une deuxième longueur d'onde optique différente de la première longueur d'onde ; et
 - un module de calcul (40) comprenant une mémoire (42) et un processeur (44) agencé pour exécuter un programme d'instructions stocké dans la mémoire pour :

- mesurer la photoréfraction de l'œil (2) à la première longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec la première lumière (20) ; 5
- mesurer la photoréfraction de l'œil (2) à la deuxième longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec une deuxième lumière (22) ; 10
- déterminer la prescription pour l'œil (2) sur la base de la photoréfraction mesurée à la première longueur d'onde et de la photoréfraction mesurée à la deuxième longueur d'onde, 15

le procédé comprenant au moins :

- la mesure de la photoréfraction de l'œil à la première longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec la première lumière émise successivement par la ou chaque première source de lumière (16) ; 20
 - mesurer la photoréfraction de l'œil à la deuxième longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec la deuxième lumière émise par la deuxième source de lumière (18) ; et 25
 - déterminer la prescription pour l'œil sur la base de la photoréfraction mesurée à la première longueur d'onde et de la photoréfraction mesurée à la deuxième longueur d'onde. 30
- 12.** Procédé selon la revendication 11, comprenant en outre la détermination de la distance entre l'œil (2) de la personne et la caméra (30). 35
- 13.** Procédé de fourniture d'une lentille ophtalmique adaptée à une prescription du porteur, le procédé comprenant : 40
- la détermination d'une prescription pour un œil du porteur selon l'une quelconque des revendications précédentes 11 ou 12 ; et 45
 - la fabrication de la lentille ophtalmique selon la prescription déterminée adaptée à l'œil du porteur.
- 14.** Produit de programme informatique comprenant une ou plusieurs séquences d'instructions stockées qui sont accessibles à un processeur et qui, lorsqu'elles sont exécutées par le processeur, amènent le processeur à effectuer au moins les étapes de : 50
- mesure de la photoréfraction d'un œil à une première longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de 55

l'éclairage de l'œil avec la première lumière émise par la ou chaque première source de lumière ;

- mesure de la photoréfraction de l'œil à une deuxième longueur d'onde sur la base d'au moins une image de l'œil enregistrée lors de l'éclairage de l'œil avec une deuxième lumière émise par une deuxième source de lumière ;
- détermination d'une prescription pour l'œil sur la base de la photoréfraction mesurée à la première longueur d'onde et de la photoréfraction mesurée à la deuxième longueur d'onde.

- 15.** Support lisible par ordinateur exécutant une ou plusieurs séquences d'instructions du produit de programme informatique selon la revendication 14.

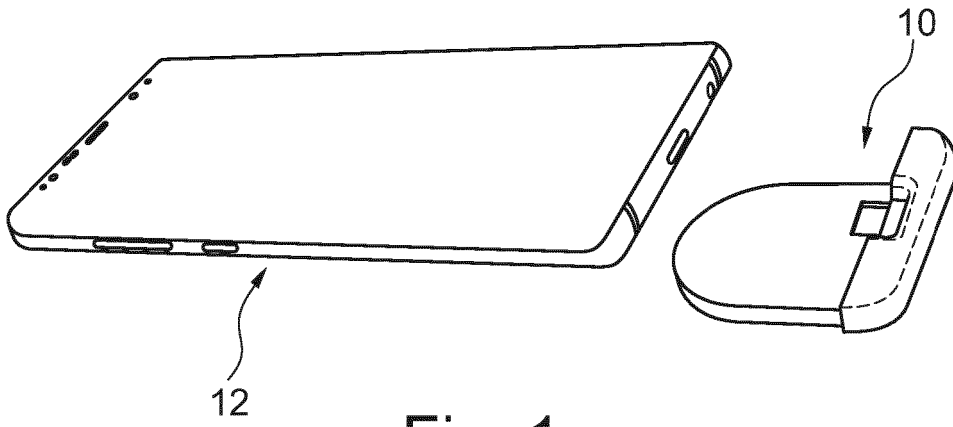


Fig. 1

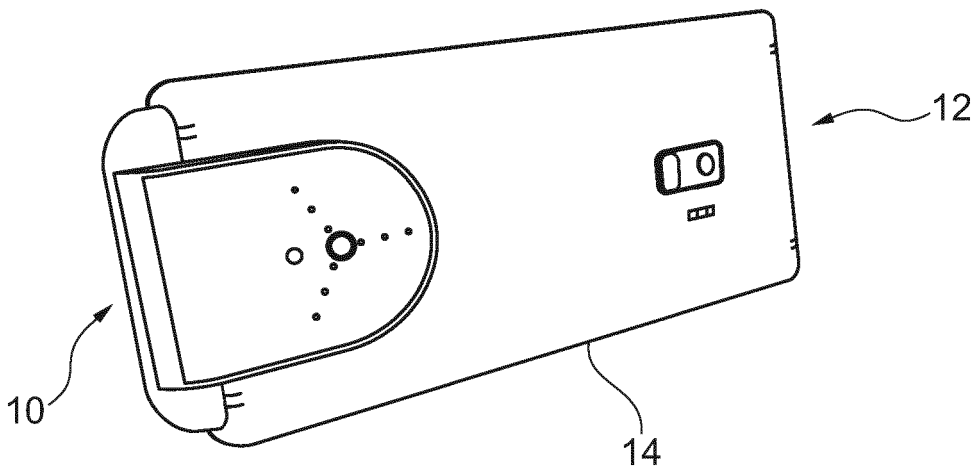


Fig. 2

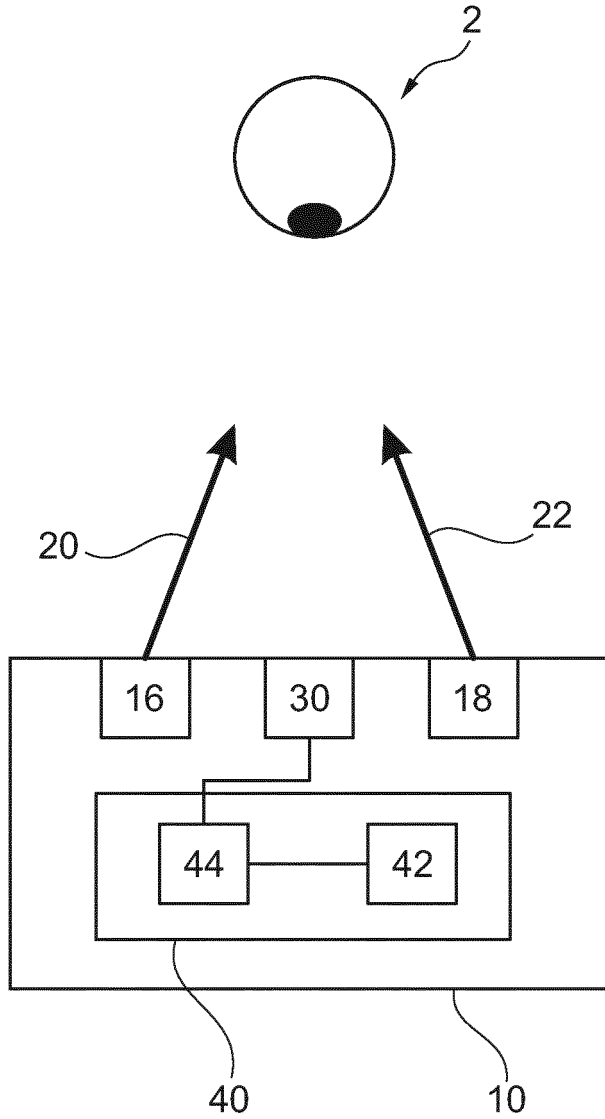


Fig. 3

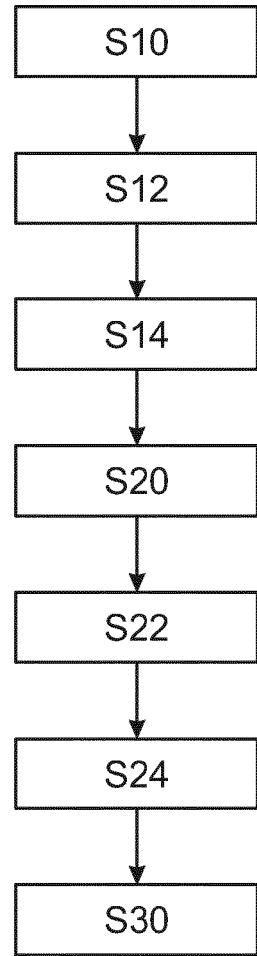


Fig. 4

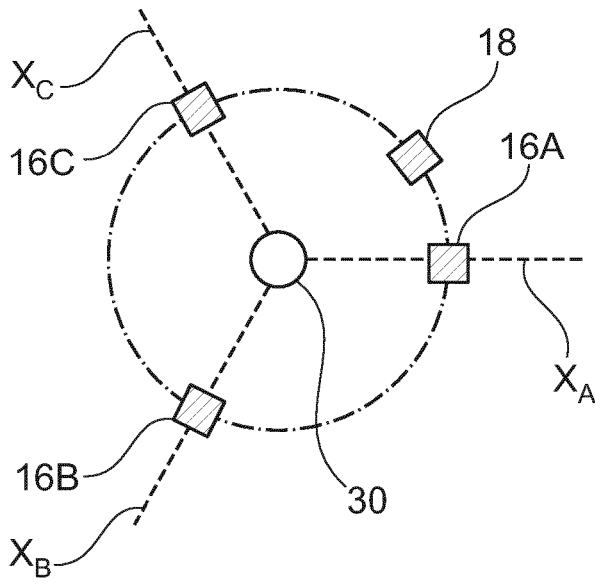


Fig. 5

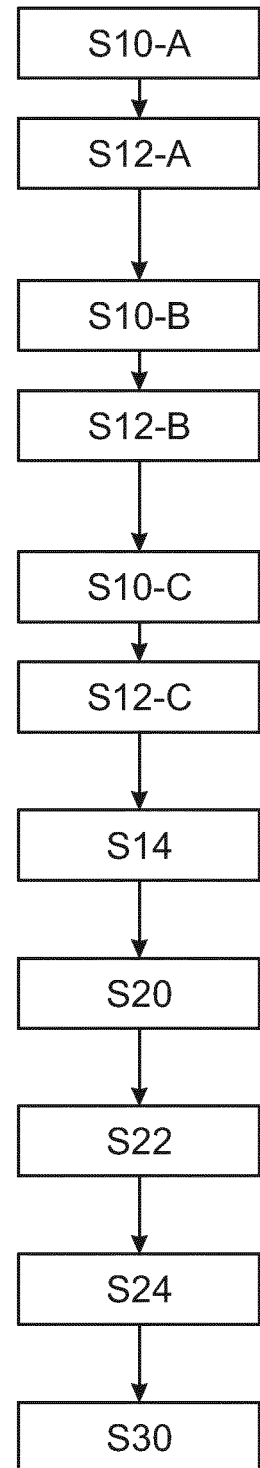


Fig. 6

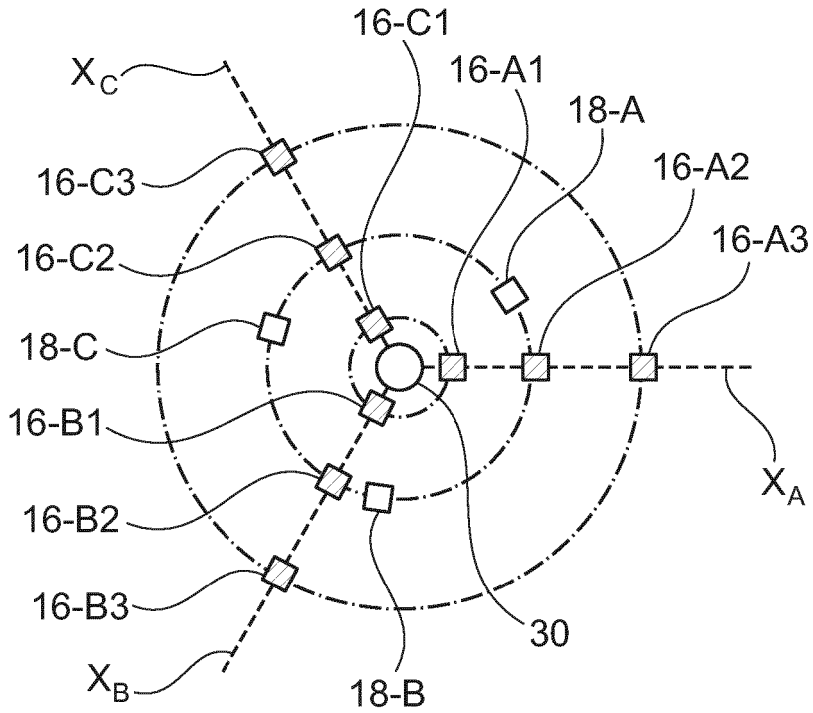


Fig. 7

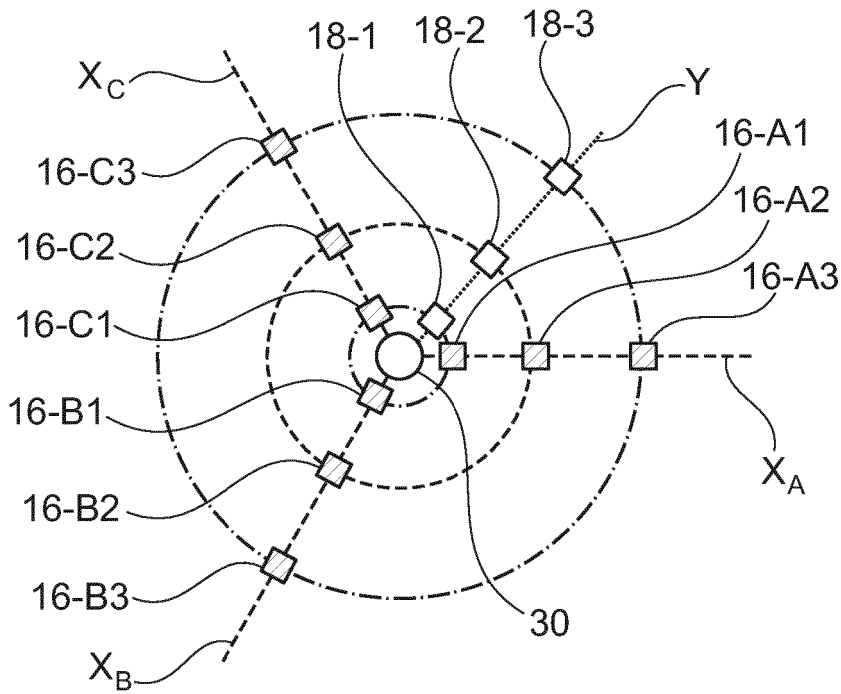


Fig. 9

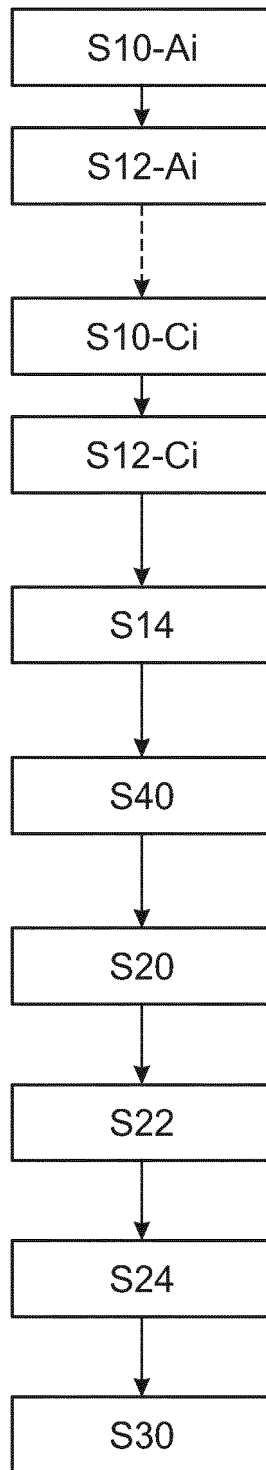


Fig. 8

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- WO 2019099952 A1 [0002]
- WO 2012177544 A1 [0002]
- US 2017150882 A1 [0002]

Non-patent literature cited in the description

- **Y. WU ; L.N. THIBOS ; T.R. CANDY.** Two-dimensional simulation of eccentric photorefractive images for ametropes: factors influencing the measurement. *Ophthalmic Physiol. Opt.*, 2018, vol. 38, 432-446 [0005]