



(12) **United States Patent**  
**Reiley**

(10) **Patent No.:** **US 9,743,969 B2**  
(45) **Date of Patent:** **Aug. 29, 2017**

(54) **SYSTEMS AND METHODS FOR THE  
FIXATION OR FUSION OF BONE**

(71) Applicant: **SI-Bone Inc.**, San Jose, CA (US)  
(72) Inventor: **Mark A. Reiley**, Washington, DC (US)  
(73) Assignee: **SI-Bone Inc.**, San Jose, CA (US)  
(\* ) Notice: Subject to any disclaimer, the term of this patent is extended or adjusted under 35 U.S.C. 154(b) by 0 days.

(21) Appl. No.: **14/245,759**

(22) Filed: **Apr. 4, 2014**

(65) **Prior Publication Data**  
US 2014/0222150 A1 Aug. 7, 2014

**Related U.S. Application Data**

(60) Continuation of application No. 14/162,689, filed on Jan. 23, 2014, now Pat. No. 8,840,623, which is a (Continued)

(51) **Int. Cl.**  
**A61B 17/58** (2006.01)  
**A61B 17/60** (2006.01)  
(Continued)

(52) **U.S. Cl.**  
CPC ..... **A61B 17/864** (2013.01); **A61B 17/1615** (2013.01); **A61B 17/68** (2013.01); **A61B 17/70** (2013.01); **A61B 17/846** (2013.01); **A61B 17/866** (2013.01); **A61B 17/8625** (2013.01); **A61B 17/8685** (2013.01); **A61F 2/4455** (2013.01); **A61F 2/0077** (2013.01); **A61F 2/28** (2013.01); **A61F 2/30767** (2013.01); **A61F 2/447** (2013.01); **A61F 2/4465** (2013.01); **A61F 2002/305** (2013.01); **A61F 2002/3023** (2013.01);  
(Continued)

(58) **Field of Classification Search**  
CPC .... A61B 17/025; A61F 2/4603; A61F 2/4614; A61F 2002/4631; A61F 2/4644  
USPC ..... 606/246-279, 62, 86 A, 86 R, 99, 104, 606/105  
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

1,951,278 A 3/1934 Ericsson  
2,136,471 A 11/1938 Schneider  
(Continued)

FOREIGN PATENT DOCUMENTS

CN 1128944 A 8/1996  
CN 1190882 A 8/1998  
(Continued)

OTHER PUBLICATIONS


Reiley, Mark A.; U.S. Appl. No. 12/357,483 entitled "Systems and methods for the fixation or fusion of bone in the hand and wrist," filed Jan. 22, 2009 (abandoned).  
(Continued)

*Primary Examiner* — Ellen C Hammond  
*Assistant Examiner* — Christina Negrelli-rodrique  
(74) *Attorney, Agent, or Firm* — Shay Glenn LLP

(57) **ABSTRACT**

A joint between two bone segments is fused by passing an elongated, rectilinear bone fusion device over a guide pin across the joint and into tight engagement within bores formed in the bone segments, to thereby restrict movement of the elongated bone fusion device across the joint. The elongated, rectilinear bone fusion device also provides bony in-growth within the bores along the exterior surface of the bone fusion device.

**10 Claims, 11 Drawing Sheets**

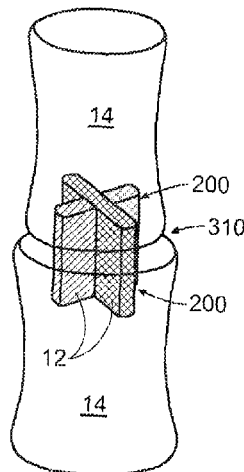

**Related U.S. Application Data**

continuation of application No. 13/078,530, filed on Apr. 1, 2011, now Pat. No. 9,561,063, which is a continuation of application No. 12/804,516, filed on Jul. 22, 2010, now Pat. No. 8,202,305, which is a division of application No. 11/136,141, filed on May 24, 2005, now Pat. No. 7,922,765, which is a continuation-in-part of application No. 10/914,629, filed on Aug. 9, 2004, now abandoned.

(51) **Int. Cl.**

- A61F 2/00* (2006.01)
- A61B 17/86* (2006.01)
- A61B 17/16* (2006.01)
- A61B 17/68* (2006.01)
- A61F 2/44* (2006.01)
- A61B 17/84* (2006.01)
- A61B 17/70* (2006.01)
- A61F 2/28* (2006.01)
- A61F 2/30* (2006.01)
- A61F 2/42* (2006.01)

(52) **U.S. Cl.**

- CPC ..... *A61F 2002/30062* (2013.01); *A61F 2002/3082* (2013.01); *A61F 2002/3085* (2013.01); *A61F 2002/30156* (2013.01); *A61F 2002/30179* (2013.01); *A61F 2002/30235* (2013.01); *A61F 2002/30405* (2013.01); *A61F 2002/30576* (2013.01); *A61F 2002/30604* (2013.01); *A61F 2002/30622* (2013.01); *A61F 2002/30777* (2013.01); *A61F 2002/30785* (2013.01); *A61F 2002/30787* (2013.01); *A61F 2002/30841* (2013.01); *A61F 2002/4238* (2013.01); *A61F 2002/448* (2013.01); *A61F 2210/0004* (2013.01); *A61F 2220/0025* (2013.01); *A61F 2230/0023* (2013.01); *A61F 2230/0058* (2013.01); *A61F 2230/0069* (2013.01); *A61F 2310/00017* (2013.01); *A61F 2310/00023* (2013.01); *A61F 2310/00029* (2013.01); *A61F 2310/0097* (2013.01); *A61F 2310/00131* (2013.01); *A61F 2310/00179* (2013.01); *A61F 2310/00329* (2013.01); *A61F 2310/00353* (2013.01); *A61F 2310/00359* (2013.01); *A61F 2310/00796* (2013.01)

(56)

**References Cited**

U.S. PATENT DOCUMENTS

2,243,717	A	5/1941	Moreira	
2,414,882	A	7/1947	Longfellow	
2,562,419	A	7/1951	Ferris	
2,675,801	A	4/1954	Bambara et al.	
2,697,433	A	12/1954	Zehnder	
3,076,453	A	2/1963	Tronzo	
3,506,982	A	4/1970	Steffee	
3,694,821	A	10/1972	Moritz	
3,709,218	A	1/1973	Halloran	
3,744,488	A *	7/1973	Cox	<i>A61B 17/72</i> 606/309
4,059,115	A	11/1977	Jumashev et al.	
4,156,943	A	6/1979	Collier	
4,292,964	A	10/1981	Ulrich	
4,341,206	A	7/1982	Perrett et al.	
4,344,190	A	8/1982	Lee et al.	
4,399,813	A	8/1983	Barber	
4,423,721	A	1/1984	Otte et al.	
4,475,545	A	10/1984	Ender	
4,501,269	A	2/1985	Bagby	
4,569,338	A	2/1986	Edwards	

4,612,918	A	9/1986	Slocum	
4,622,959	A	11/1986	Marcus	
4,630,601	A	12/1986	Harder et al.	
4,638,799	A	1/1987	Moore	
4,657,550	A	4/1987	Daher	
4,743,256	A	5/1988	Brantigan	
4,773,402	A	9/1988	Asher et al.	
4,787,378	A	11/1988	Sodhi	
4,790,303	A	12/1988	Steffee	
4,834,757	A	5/1989	Brantigan	
4,846,162	A	7/1989	Moehring	
4,877,019	A	10/1989	Vives	
4,878,915	A	11/1989	Brantigan	
4,898,186	A	2/1990	Ikada et al.	
4,904,261	A	2/1990	Dove et al.	
4,950,270	A	8/1990	Bowman et al.	
4,961,740	A	10/1990	Ray et al.	
4,981,481	A	1/1991	Kranz et al.	
5,034,011	A	7/1991	Howland	
5,034,013	A	7/1991	Kyle et al.	
5,035,697	A	7/1991	Frigg	
5,041,118	A	8/1991	Wasilewski	
5,053,035	A	10/1991	McClaren	
5,059,193	A	10/1991	Kuslich	
5,066,296	A	11/1991	Chapman et al.	
5,102,414	A	4/1992	Kirsch	
5,108,397	A	4/1992	White	
5,122,141	A	6/1992	Simpson et al.	
5,139,498	A	8/1992	Astudillo Ley	
5,139,500	A	8/1992	Schwartz	
5,147,367	A	9/1992	Ellis	
5,147,402	A	9/1992	Bohler et al.	
5,190,551	A	3/1993	Chin et al.	
5,197,961	A	3/1993	Castle	
5,242,444	A	9/1993	MacMillan	
5,298,254	A	3/1994	Prewett et al.	
5,334,205	A	8/1994	Cain	
5,380,325	A	1/1995	Lahille et al.	
5,390,683	A	2/1995	Pisharodi	
5,433,718	A	7/1995	Brinker	
5,443,466	A	8/1995	Shah	
5,458,638	A	10/1995	Kuslich et al.	
5,470,334	A	11/1995	Ross et al.	
5,480,402	A	1/1996	Kim	
5,569,249	A	10/1996	James et al.	
5,591,235	A	1/1997	Kuslich	
5,593,409	A	1/1997	Michelson	
5,609,636	A	3/1997	Kohrs et al.	
5,626,616	A	5/1997	Speece	
5,643,264	A	7/1997	Sherman et al.	
5,645,599	A	7/1997	Samani	
5,658,337	A	8/1997	Kohrs et al.	
5,667,510	A	9/1997	Combs	
5,669,909	A	9/1997	Zdeblick et al.	
5,672,178	A	9/1997	Petersen	
5,683,391	A	11/1997	Boyd	
5,709,683	A	1/1998	Bagby	
5,713,904	A	2/1998	Errico et al.	
5,716,358	A	2/1998	Ochoa et al.	
5,725,581	A	3/1998	Bränemark	
5,743,912	A	4/1998	LaHille et al.	
5,759,035	A	6/1998	Ricci	
5,766,174	A	6/1998	Perry	
5,766,261	A	6/1998	Neal et al.	
5,788,699	A	8/1998	Bobst et al.	
5,800,440	A	9/1998	Stead	
5,868,749	A	2/1999	Reed	
5,897,556	A	4/1999	Drewry et al.	
5,928,239	A	7/1999	Mirza	
5,941,885	A	8/1999	Jackson	
5,961,522	A	10/1999	Mehdizadeh	
5,961,554	A	10/1999	Janson et al.	
6,010,507	A	1/2000	Rudloff	
6,015,409	A	1/2000	Jackson	
6,053,916	A	4/2000	Moore	
6,056,749	A	5/2000	Kuslich	
6,086,589	A	7/2000	Kuslich et al.	
6,096,080	A	8/2000	Nicholson et al.	
6,120,504	A	9/2000	Brumback et al.	

(56)

References Cited

U.S. PATENT DOCUMENTS

6,143,031	A	11/2000	Knothe et al.	8,062,365	B2	11/2011	Schwab
6,197,062	B1	3/2001	Fenlin	8,066,705	B2	11/2011	Michelson
6,210,442	B1	4/2001	Wing et al.	8,066,709	B2	11/2011	Michelson
6,214,049	B1	4/2001	Gayer et al.	8,142,481	B2	3/2012	Warnick
6,221,074	B1	4/2001	Cole et al.	8,202,305	B2	6/2012	Reiley
6,224,607	B1	5/2001	Michelson	8,308,779	B2	11/2012	Reiley
6,241,732	B1	6/2001	Overaker et al.	8,388,667	B2	3/2013	Reiley et al.
6,264,657	B1	7/2001	Urbahns et al.	8,414,648	B2	4/2013	Reiley
6,270,528	B1	8/2001	McKay	8,425,570	B2	4/2013	Reiley
6,287,343	B1	9/2001	Kuslich et al.	8,444,693	B2	5/2013	Reiley
6,302,885	B1	10/2001	Essiger	8,470,004	B2	6/2013	Reiley
6,302,914	B1	10/2001	Michelson	8,672,986	B2	3/2014	Klaue et al.
6,306,140	B1	10/2001	Siddiqui	8,734,462	B2	5/2014	Reiley et al.
6,319,253	B1	11/2001	Ackeret et al.	8,945,190	B2	2/2015	Culbert et al.
6,406,498	B1	6/2002	Tormala et al.	2001/0012942	A1	8/2001	Estes et al.
6,409,768	B1	6/2002	Tepic et al.	2001/0046518	A1	11/2001	Sawhney
6,451,020	B1	9/2002	Zucherman et al.	2001/0047207	A1	11/2001	Michelson
6,471,707	B1	10/2002	Miller et al.	2001/0049529	A1	12/2001	Cachia et al.
6,485,518	B1	11/2002	Cornwall et al.	2002/0038123	A1	3/2002	Visotsky et al.
6,497,707	B1	12/2002	Bowman et al.	2002/0049497	A1	4/2002	Mason
6,517,541	B1	2/2003	Sesic	2002/0077641	A1	6/2002	Michelson
6,520,969	B2	2/2003	Lambrech et al.	2002/0082598	A1	6/2002	Teitelbaum
6,524,314	B1	2/2003	Dean et al.	2002/0120275	A1	8/2002	Schmieding et al.
6,527,775	B1	3/2003	Warburton	2002/0128652	A1	9/2002	Ferree
6,558,386	B1*	5/2003	Cragg ..... A61B 17/1642 606/279	2002/0143334	A1	10/2002	von Hoffmann et al.
6,565,566	B1	5/2003	Wagner et al.	2002/0143335	A1	10/2002	von Hoffmann et al.
6,575,899	B1	6/2003	Foley et al.	2002/0151903	A1	10/2002	Takei et al.
6,575,991	B1	6/2003	Chesbrough et al.	2002/0169507	A1	11/2002	Malone
6,579,293	B1	6/2003	Chandran	2002/0183858	A1	12/2002	Contiliano et al.
6,582,431	B1	6/2003	Ray	2002/0198527	A1	12/2002	Mückter
6,595,998	B2	7/2003	Johnson et al.	2003/0018336	A1	1/2003	Vandewalle
6,602,293	B1	8/2003	Biermann et al.	2003/0032961	A1	2/2003	Pelo et al.
6,605,090	B1	8/2003	Trieu et al.	2003/0050642	A1	3/2003	Schmieding et al.
6,607,530	B1	8/2003	Carl et al.	2003/0065332	A1	4/2003	TenHuisen et al.
6,620,163	B1	9/2003	Michelson	2003/0074000	A1	4/2003	Roth et al.
6,635,059	B2	10/2003	Randall et al.	2003/0078660	A1	4/2003	Clifford et al.
6,666,868	B2	12/2003	Fallin	2003/0083668	A1	5/2003	Rogers et al.
6,669,529	B1	12/2003	Scaries	2003/0083688	A1	5/2003	Simonson
6,673,075	B2	1/2004	Santilli	2003/0097131	A1	5/2003	Schon et al.
6,692,501	B2	2/2004	Michelson	2003/0139815	A1	7/2003	Grooms et al.
6,723,099	B1	4/2004	Goshert	2003/0181982	A1	9/2003	Kuslich
6,740,118	B2	5/2004	Eisermann et al.	2003/0199983	A1	10/2003	Michelson
6,743,257	B2	6/2004	Castro	2003/0229358	A1	12/2003	Errico et al.
D493,533	S	7/2004	Blain	2003/0233146	A1	12/2003	Grinberg et al.
6,793,656	B1	9/2004	Mathews	2003/0233147	A1	12/2003	Nicholson et al.
6,827,740	B1	12/2004	Michelson	2004/0010315	A1	1/2004	Song
6,984,235	B2*	1/2006	Huebner ..... 470/10	2004/0024458	A1	2/2004	Senegas et al.
6,991,461	B2	1/2006	Gittleman	2004/0034422	A1	2/2004	Errico et al.
7,118,579	B2	10/2006	Michelson	2004/0073216	A1	4/2004	Lieberman
7,175,663	B1	2/2007	Stone	2004/0073314	A1	4/2004	White et al.
7,211,085	B2	5/2007	Michelson	2004/0082955	A1	4/2004	Zirkle
7,223,269	B2	5/2007	Chappuis	2004/0087948	A1	5/2004	Suddaby
7,314,488	B2	1/2008	Reiley	2004/0097927	A1	5/2004	Yeung et al.
7,335,205	B2	2/2008	Aeschlimann et al.	2004/0106925	A1	6/2004	Culbert
7,338,500	B2	3/2008	Chappuis	2004/0117022	A1	6/2004	Marnay et al.
7,452,359	B1	11/2008	Michelson	2004/0127990	A1	7/2004	Bartish, Jr. et al.
7,452,369	B2	11/2008	Barry	2004/0138750	A1	7/2004	Mitchell
7,481,831	B2	1/2009	Bonutti	2004/0138753	A1	7/2004	Ferree
7,527,649	B1	5/2009	Blain	2004/0147929	A1	7/2004	Biedermann et al.
7,534,254	B1	5/2009	Michelson	2004/0176287	A1	9/2004	Harrison et al.
7,537,616	B1	5/2009	Branch et al.	2004/0176853	A1	9/2004	Sennett et al.
7,569,054	B2	8/2009	Michelson	2004/0181282	A1	9/2004	Zucherman et al.
7,569,059	B2	8/2009	Cerundolo	2004/0210221	A1	10/2004	Kozak et al.
7,601,155	B2	10/2009	Petersen	2004/0220574	A1*	11/2004	Pelo ..... A61F 2/0063 606/232
7,648,509	B2	1/2010	Stark	2004/0225360	A1	11/2004	Malone
7,686,805	B2	3/2010	Michelson	2004/0230305	A1	11/2004	Gorensek et al.
7,699,852	B2	4/2010	Frankel et al.	2004/0260286	A1	12/2004	Ferree
7,708,761	B2	5/2010	Petersen	2004/0267369	A1	12/2004	Lyons et al.
7,758,646	B2	7/2010	Khandkar et al.	2005/0015059	A1	1/2005	Sweeney
7,857,832	B2	12/2010	Culbert et al.	2005/0015146	A1	1/2005	Louis et al.
7,887,565	B2	2/2011	Michelson	2005/0033435	A1	2/2005	Belliard et al.
7,909,832	B2	3/2011	Michelson	2005/0049590	A1	3/2005	Alleyne et al.
7,922,765	B2	4/2011	Reiley	2005/0055023	A1	3/2005	Sohngen et al.
7,942,879	B2	5/2011	Christie et al.	2005/0075641	A1	4/2005	Singhatat et al.
				2005/0080415	A1	4/2005	Keyer et al.
				2005/0107878	A1	5/2005	Conchy
				2005/0124993	A1	6/2005	Chappuis
				2005/0131409	A1	6/2005	Chervitz et al.

(56)

References Cited

U.S. PATENT DOCUMENTS

2005/0137605 A1 6/2005 Assell et al.  
 2005/0149192 A1 7/2005 Zucherman et al.  
 2005/0159749 A1 7/2005 Levy et al.  
 2005/0165398 A1 7/2005 Reiley  
 2005/0192572 A1 9/2005 Abdelgany et al.  
 2005/0228384 A1 10/2005 Zucherman et al.  
 2005/0246021 A1 11/2005 Ringeisen et al.  
 2005/0251146 A1 11/2005 Martz et al.  
 2005/0277940 A1 12/2005 Neff  
 2006/0036247 A1 2/2006 Michelson  
 2006/0036251 A1 2/2006 Reiley  
 2006/0054171 A1 3/2006 Dall  
 2006/0058793 A1 3/2006 Michelson  
 2006/0058800 A1 3/2006 Ainsworth et al.  
 2006/0062825 A1 3/2006 Maccellini  
 2006/0084986 A1 4/2006 Grinberg et al.  
 2006/0089656 A1 4/2006 Allard et al.  
 2006/0111779 A1 5/2006 Petersen  
 2006/0129247 A1 6/2006 Brown et al.  
 2006/0142772 A1 6/2006 Ralph et al.  
 2006/0161163 A1 7/2006 Shino  
 2006/0178673 A1 8/2006 Curran  
 2006/0217717 A1 9/2006 Whipple  
 2006/0241776 A1 10/2006 Brown et al.  
 2006/0271054 A1 11/2006 Sucec et al.  
 2007/0066977 A1 3/2007 Assell et al.  
 2007/0083265 A1 4/2007 Malone  
 2007/0149976 A1 6/2007 Hale et al.  
 2007/0156144 A1 7/2007 Ulrich et al.  
 2007/0156241 A1 7/2007 Reiley et al.  
 2007/0156246 A1 7/2007 Meswania et al.  
 2007/0219634 A1 9/2007 Greenhalgh et al.  
 2008/0065093 A1 3/2008 Assell et al.  
 2008/0065215 A1 3/2008 Reiley  
 2008/0109083 A1 5/2008 Van Hoeck et al.  
 2009/0043393 A1 2/2009 Duggal et al.  
 2009/0259261 A1 10/2009 Reiley  
 2009/0324678 A1 12/2009 Thorne et al.  
 2010/0094295 A1 4/2010 Schnieders et al.  
 2010/0106194 A1 4/2010 Bonutti et al.  
 2010/0106195 A1 4/2010 Serhan et al.  
 2010/0145461 A1 6/2010 Landry et al.  
 2010/0191292 A1 7/2010 DeMeo et al.  
 2010/0280622 A1 11/2010 McKinley  
 2011/0029019 A1 2/2011 Ainsworth et al.  
 2011/0040362 A1 2/2011 Godara et al.  
 2011/0060375 A1 3/2011 Bonutti  
 2011/0087294 A1 4/2011 Reiley  
 2011/0118796 A1 5/2011 Reiley et al.  
 2011/0153018 A1 6/2011 Walters et al.  
 2011/0184478 A1 7/2011 Reiley  
 2012/0083887 A1 4/2012 Purcell et al.  
 2012/0179256 A1 7/2012 Reiley  
 2013/0131739 A1 5/2013 Reiley  
 2013/0226301 A1 8/2013 Reiley  
 2013/0237988 A1 9/2013 Mauldin  
 2013/0238031 A1 9/2013 Reiley  
 2013/0238093 A1 9/2013 Mauldin et al.  
 2013/0245763 A1 9/2013 Mauldin  
 2013/0245764 A1 9/2013 Mauldin  
 2013/0253654 A1 9/2013 Reiley  
 2013/0267836 A1 10/2013 Mauldin et al.  
 2013/0267961 A1 10/2013 Mauldin et al.  
 2013/0267989 A1 10/2013 Mauldin et al.  
 2013/0289625 A1 10/2013 Reiley  
 2013/0296953 A1 11/2013 Mauldin et al.  
 2014/0257298 A1 9/2014 Reiley  
 2014/0257415 A1 9/2014 Reiley  
 2014/0330382 A1 11/2014 Mauldin

2015/0005832 A1 1/2015 Reiley  
 2015/0238205 A1 8/2015 Reiley  
 2015/0250595 A1 9/2015 Mauldin et al.

FOREIGN PATENT DOCUMENTS

CN 1909848 A 2/2007  
 EP 1287796 A1 3/2003  
 JP 59200642 A 11/1984  
 JP 05-176942 A 7/1993  
 JP 05184615 A 7/1993  
 JP 09149906 A 10/1997  
 JP 10-85231 A 4/1998  
 JP 11318931 A 11/1999  
 JP 2002509753 A 4/2002  
 JP 2003533329 A 11/2003  
 JP 2004121841 4/2004  
 JP 2004512895 4/2004  
 JP 2004516866 6/2004  
 JP 2006506181 2/2006  
 JP 2008540036 A 11/2008  
 WO WO97/31517 A2 8/1997  
 WO WO02/38054 5/2002  
 WO WO03/007839 A2 1/2003  
 WO WO2004/002344 1/2004  
 WO WO2004/043277 A1 5/2004  
 WO WO2005/009729 A2 2/2005  
 WO WO2006/003316 1/2006

OTHER PUBLICATIONS

Reiley, Mark A.; U.S. Appl. No. 14/162,689 entitled "Systems and methods for the fixation or fusion of bone," filed Jan. 23, 2014.  
 Mauldin et al.; U.S. Appl. No. 14/216,790 entitled "Systems and methods for implanting bone graft and implant," filed Mar. 17, 2014.  
 Mesiwala et al.; U.S. Appl. No. 14/216,863 entitled "Implants for spinal fixation or fusion," filed Mar. 17, 2014.  
 Yerby et al.; U.S. Appl. No. 14/216,938 entitled "Implants for facet fusion," filed Mar. 17, 2014.  
 Schneider et al.; U.S. Appl. No. 14/217,008 entitled "Systems and methods for removing an implant," filed Mar. 17, 2014.  
 Yerby et al.; U.S. Appl. No. 14/217,089 entitled "Long implant for sacroiliac joint fusion," filed Mar. 17, 2014.  
 Reiley et al.; U.S. Appl. No. 14/274,486 entitled "Systems and methods for the fixation or fusion of bone using compressive implants," filed May 9, 2014.  
 Acumed; Acutrak Headless Compression Screw (product information); 12 pgs; © 2005; retrieved Sep. 25, 2014 from <http://www.rcsed.ac.uk/fellows/Ivanrensborg/classification/surgtech/acumed/manuals/acutrak-brochure%200311.pdf>.  
 Peretz et al.; The internal bony architecture of the sacrum; Spine; 23(9); pp. 971-974; May 1, 1998.  
 Reckling et al.; U.S. Appl. No. 14/515,416 entitled "Implant Placement," filed Oct. 15, 2014.  
 Schneider et al.; U.S. Appl. No. 14/859,005 entitled "Matrix implant," filed Sep. 18, 2015.  
 Reiley et al.; U.S. Appl. No. 14/859,046 entitled "Implants for bone fixation or fusion," filed Sep. 18, 2015.  
 Lu et al.; Mechanical properties of porous materials; Journal of Porous Materials; 6(4); pp. 359-368; Nov. 1, 1999.  
 Sand et al.; U.S. Appl. No. 15/085,765 entitled "Neuromonitoring systems and methods for bone fixation or fusion procedures," filed Mar. 30, 2016.  
 Reiley et al.; U.S. Appl. No. 15/195,955 entitled "Apparatus, systems, and methods for the fixation or fusion of bone," filed Jun. 28, 2016.  
 Mauldin et al.; U.S. Appl. No. 15/208,588 entitled "System, device, and methods for joint fusion," filed Jul. 12, 2016.

\* cited by examiner

Fig. 1A

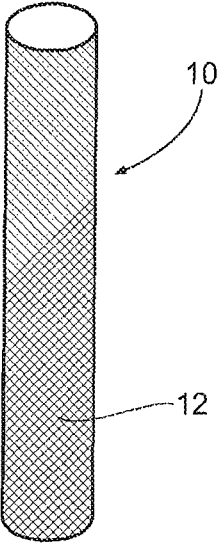


Fig. 1B

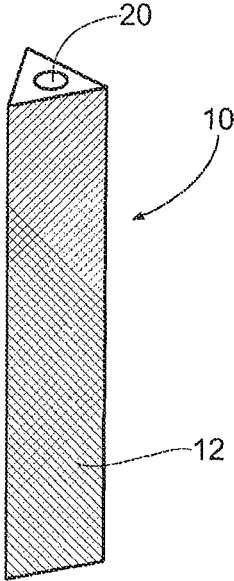


Fig. 3

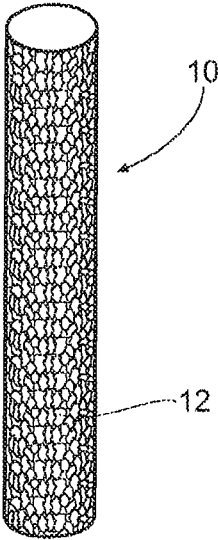
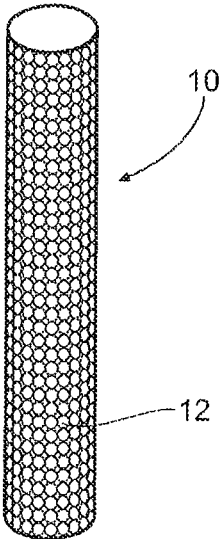


Fig. 2



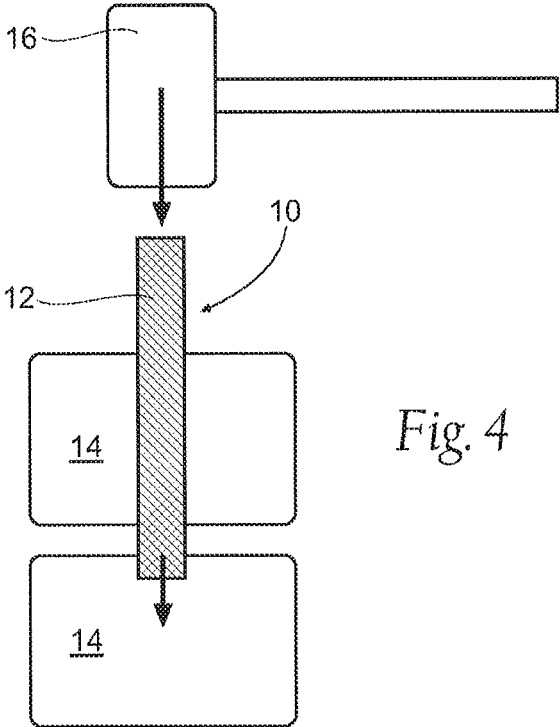


Fig. 4

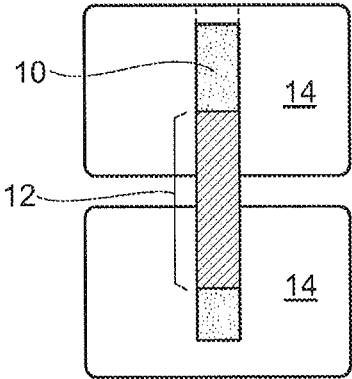


Fig. 5

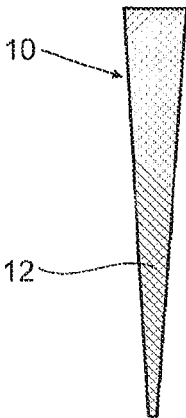


Fig. 6

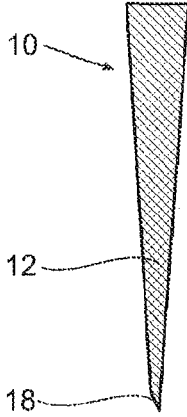


Fig. 7

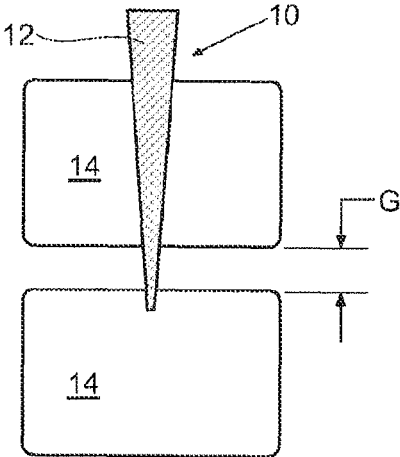


Fig. 8A

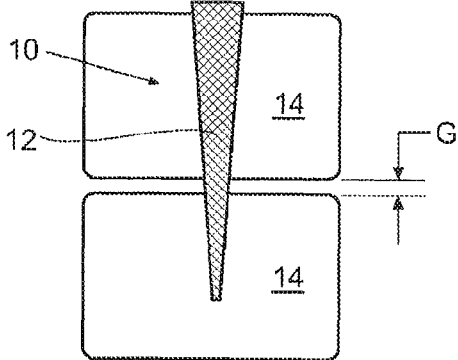


Fig. 8B

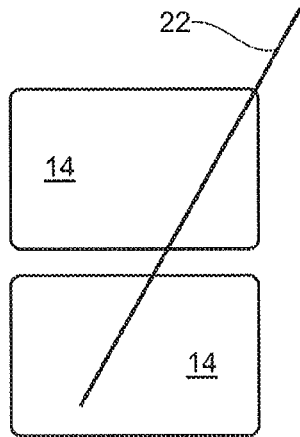


Fig. 9

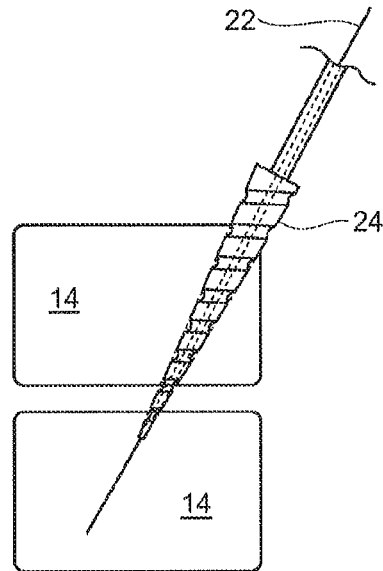


Fig. 10

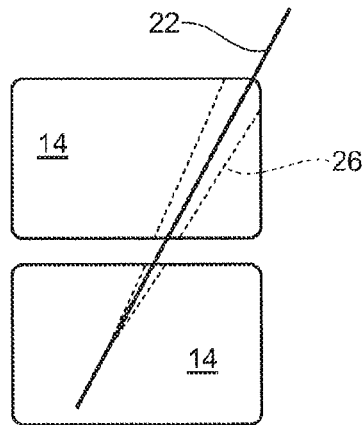


Fig. 11

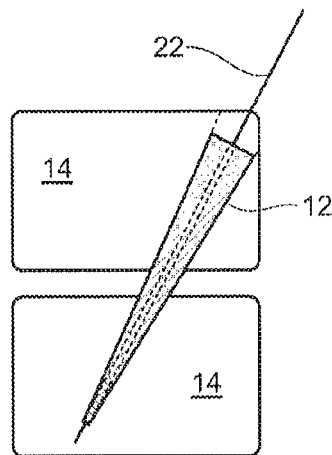
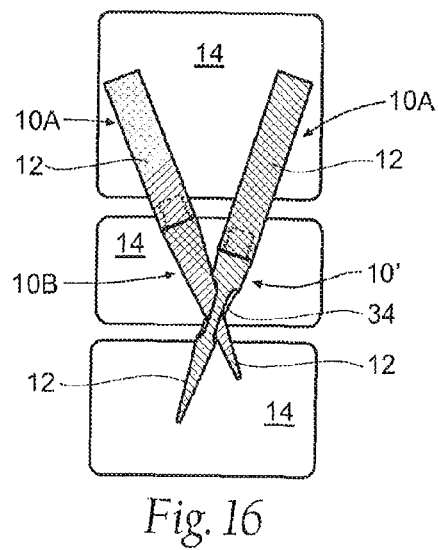
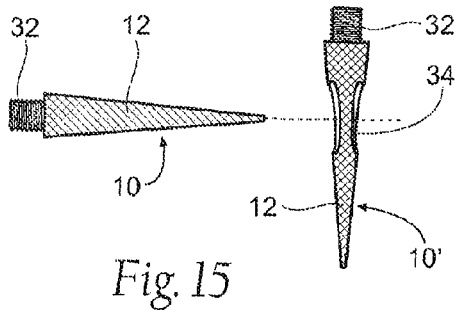
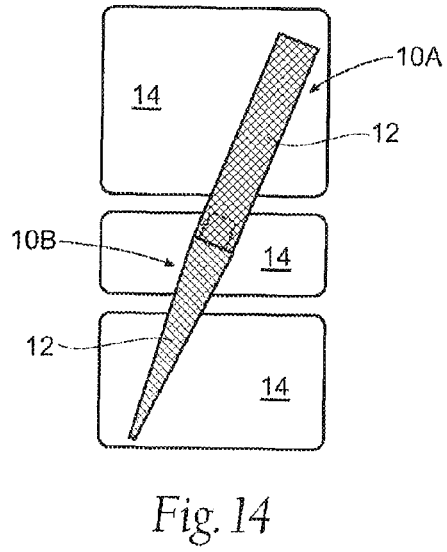
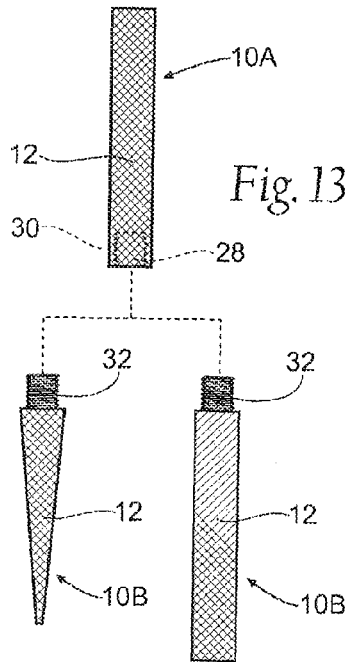


Fig. 12





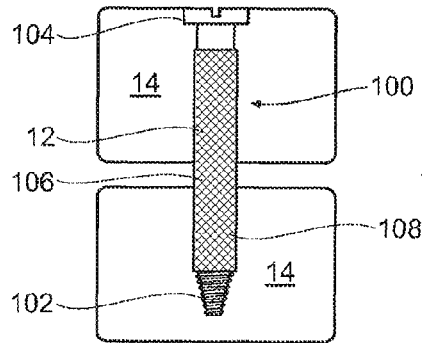


Fig. 17

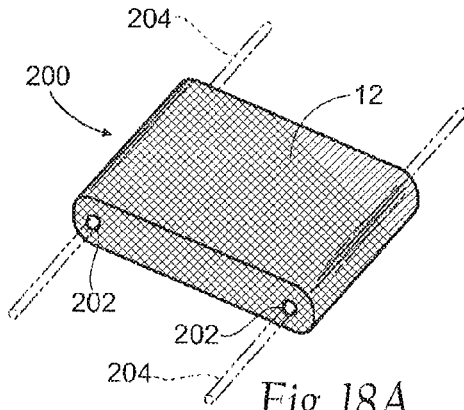


Fig. 18A

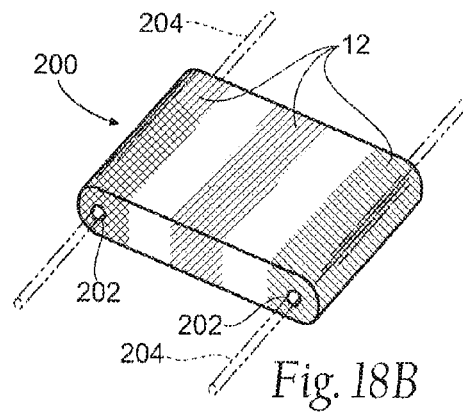


Fig. 18B

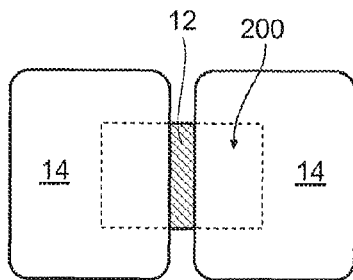


Fig. 19

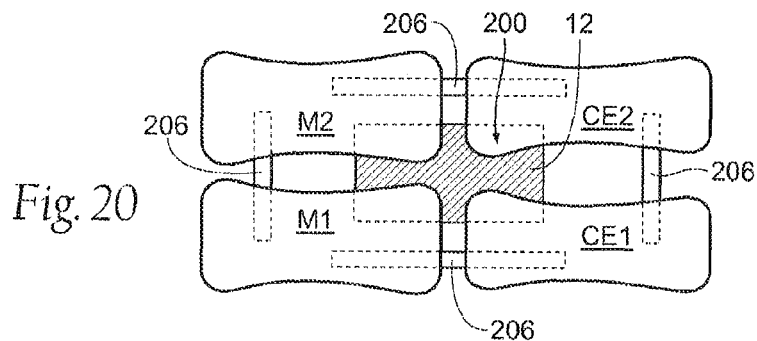


Fig. 20

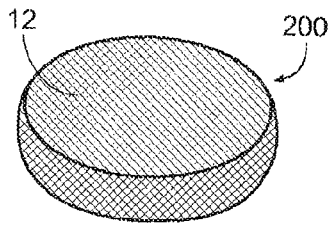


Fig. 21A

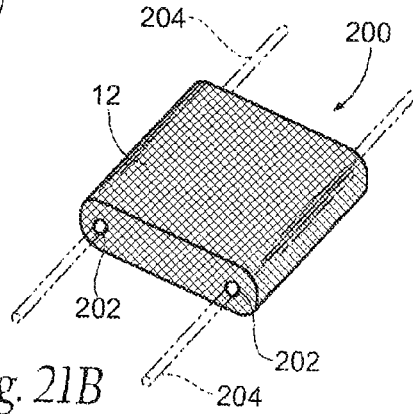


Fig. 21B




Fig. 21C

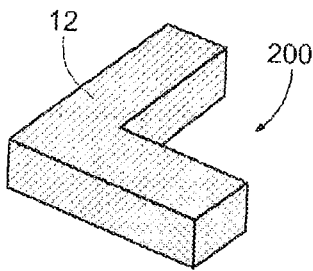


Fig. 21D

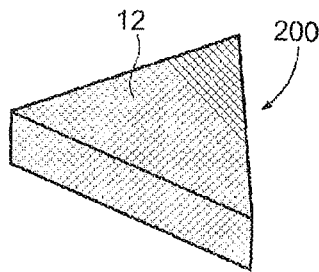


Fig. 21E

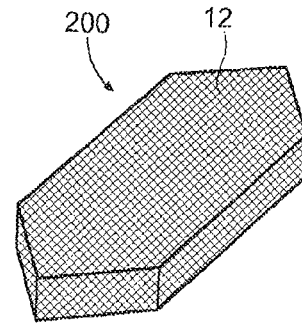


Fig. 21F

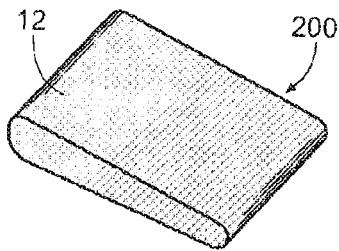


Fig. 22A

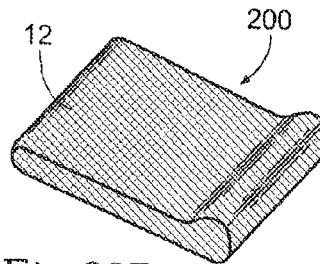
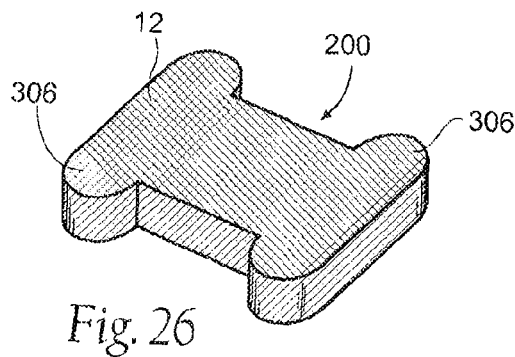
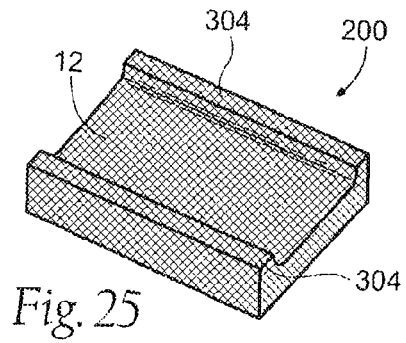
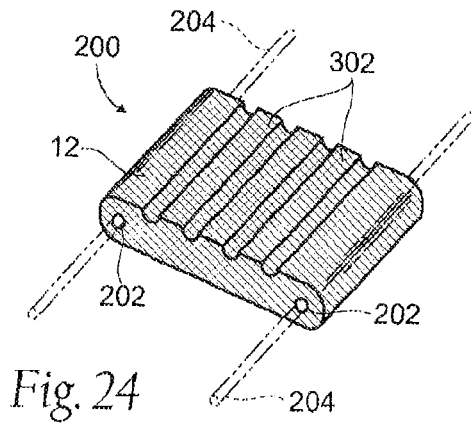
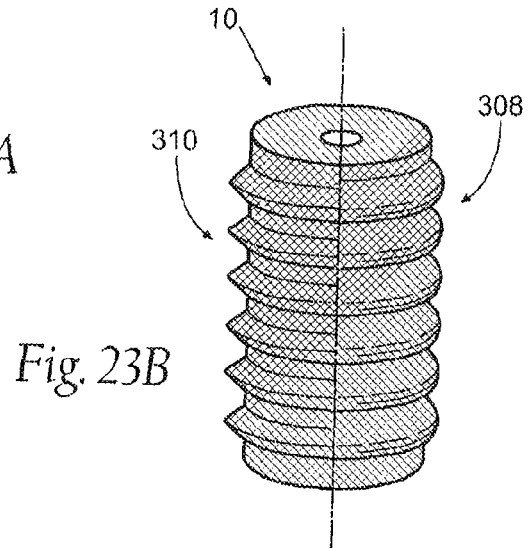
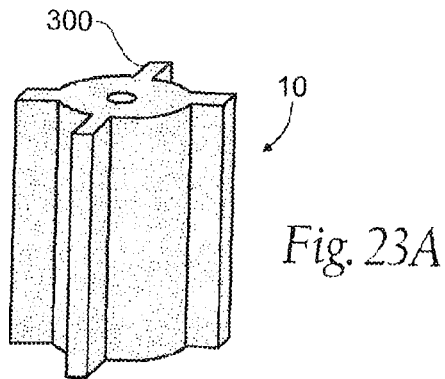


Fig. 22B



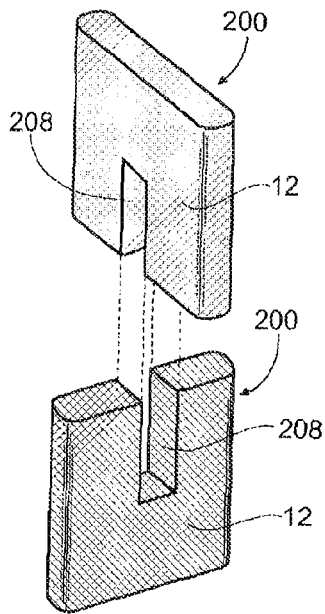


Fig. 27

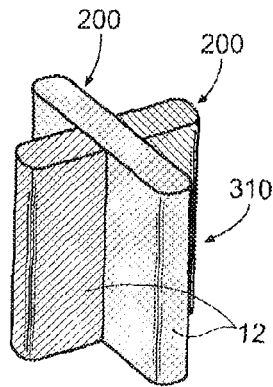


Fig. 28

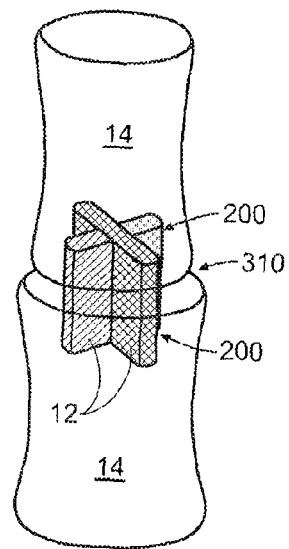


Fig. 29

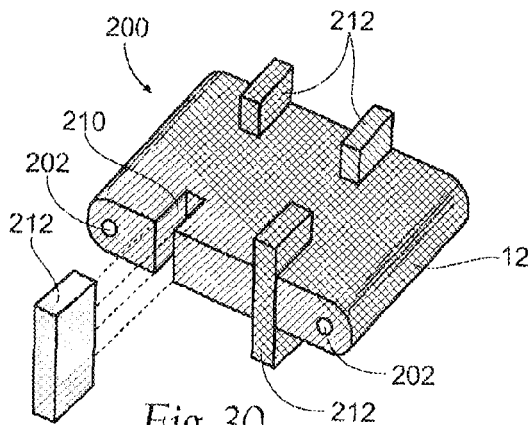


Fig. 30

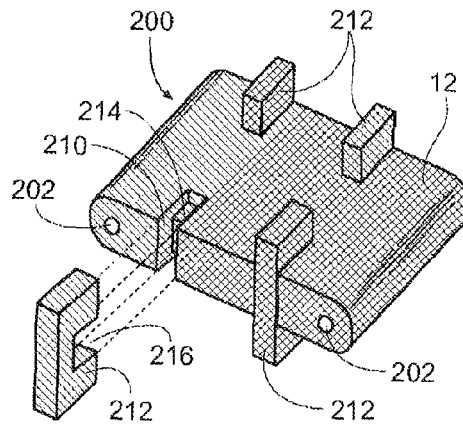
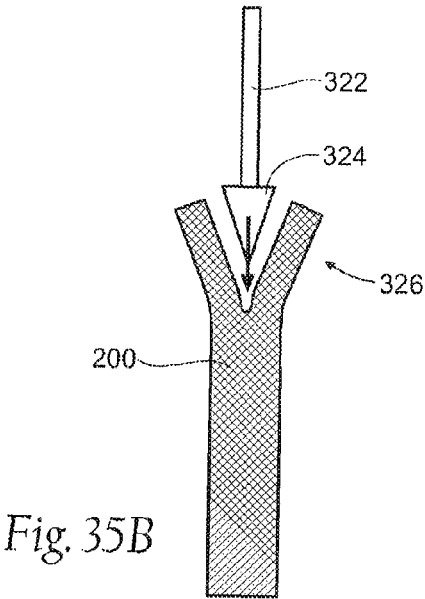
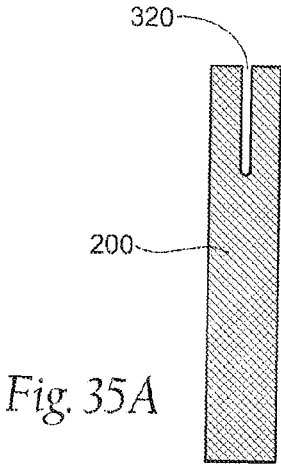
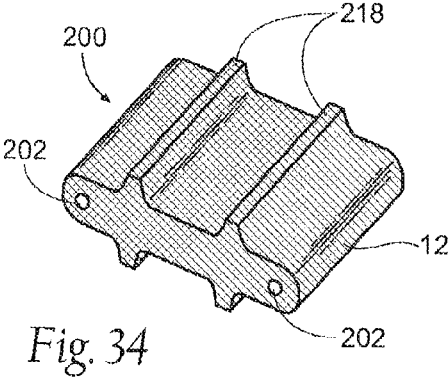
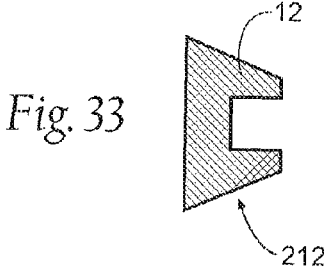
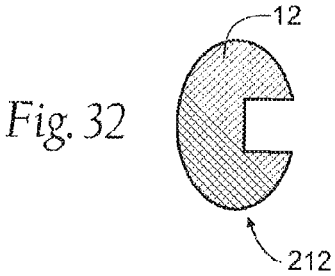


Fig. 31



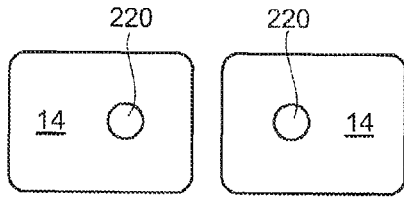


Fig. 36

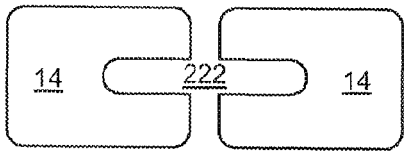


Fig. 37

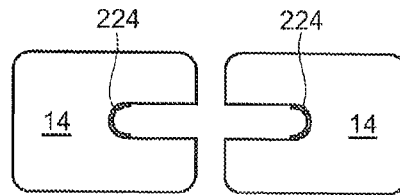


Fig. 40

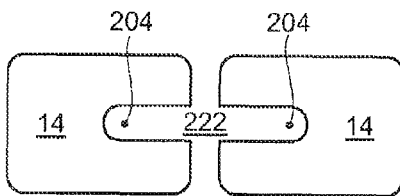


Fig. 38

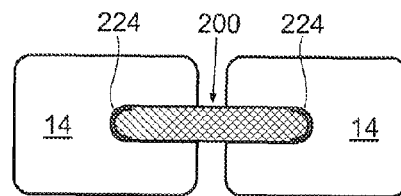


Fig. 41

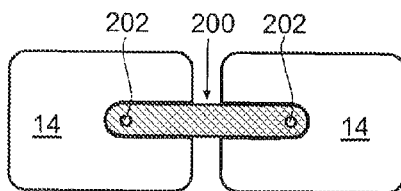


Fig. 39

1

## SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE

### CROSS REFERENCE TO RELATED APPLICATIONS

This application is a continuation of U.S. patent application Ser. No. 14/162,689, filed Jan. 23, 2014, titled "SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE," which is a continuation of U.S. patent application Ser. No. 13/078,530, filed Apr. 1, 2011, titled "SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE," now U.S. Patent Application Publication No. 2011/0184478, which is a continuation of U.S. patent application Ser. No. 12/804,516, filed Jul. 22, 2010, titled "SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE," now U.S. Pat. No. 8,202,305, which is a divisional of U.S. patent application Ser. No. 11/136,141, filed May 24, 2005, titled "SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE," now U.S. Pat. No. 7,922,765, which is a continuation-in-part of U.S. patent application Ser. No. 10/914,629, filed Aug. 9, 2004, titled "SYSTEMS AND METHODS FOR THE FIXATION OR FUSION OF BONE," now U.S. Patent Application Publication No. 2006/003625 now abandoned, each of which is herein incorporated by reference in its entirety.

### INCORPORATION BY REFERENCE

All publications and patent applications mentioned in this specification are herein incorporated by reference to the same extent as if each individual publication or patent application was specifically and individually indicated to be incorporated by reference.

### FIELD

This application relates generally to the fixation of bone.

### BACKGROUND

Many types of hardware are available both for fracture fixation and for the fixation of bones that are to fused (arthrodesed).

Metal and absorbable screws are routinely used to fixate bone fractures and osteotomies. It is important to the successful outcome of the procedure that the screw is able to generate the compressive forces helpful in promoting bone healing.

### SUMMARY OF THE DISCLOSURE

The invention provides bone fixation/fusion devices and related methods for stabilizing bone segments, which can comprise parts of the same bone (e.g., fracture fixation) or two or more individual bones (e.g., fusion). The systems and methods include a fixation/fusion device adapted for placement in association with bone segments.

One aspect of the invention provides a method comprising identifying a bone site comprising a first bone segment, a second bone segment, and a joint between the first and second bone segments. The method includes providing an elongated bone fusion device having a rectilinear cross section and including an exterior surface treated to provide bony in-growth, the elongated bone fusion device including a lumen accommodating passage over a guide pin. The

2

method includes forming a bore in the first bone segment, and forming a bore in the second bone segment that faces the bore in the first bone segment across the joint. The bores in the first and second segments are each sized and configured to tightly engage the exterior surface of the elongated bone fusion device. The method includes placing in the bore of the first bone segment a guide pin that extends across the joint into the bore of the second bone segment. The method includes fusing the joint by passing the elongated bone fusion device over the guide pin across the joint and into tight engagement within the bores of the first and second bone segments, to thereby restrict movement of the elongated bone fusion device across the joint and provide bony in-growth within the bores along the exterior surface of the bone fusion device. The method includes removing the guide pin.

Another aspect of the invention provides a joint fusion device comprising an elongated device having a rectilinear cross section free of screw threads and being sized and configured for placement in association with a joint between individual first and second bone segments in response to an axially applied, non-rotational force.

The elongated bone fusion device includes a lumen to accommodate passage over a guide pin during placement and an exterior surface treated to provide bony in-growth upon placement.

In one embodiment, the rectilinear cross section of the elongated bone fusion device comprises a square.

In one embodiment, the rectilinear cross section of the elongated bone fusion device comprises a rectangle.

In one embodiment, the rectilinear cross section of the elongated bone fusion device comprises a triangle.

### BRIEF DESCRIPTION OF THE DRAWINGS

FIGS. 1A and 1B are perspective alternative views of a bone fixation/fusion device having a bony in-growth and/or through-growth region of a mesh configuration.

FIG. 2 is a perspective view of an alternative embodiment of a bone fixation/fusion device having a bony in-growth and/or through-growth region of a beaded configuration.

FIG. 3 is a perspective view of an alternative embodiment of a bone fixation/fusion device having a bony in-growth and/or through-growth region of a trabecular configuration.

FIG. 4 is a schematic view of a bone fixation/fusion device of the type shown in FIG. 1, being inserted in association with bone across a fracture line or between different bone segments.

FIG. 5 is a schematic view of a bone fixation/fusion device positioned in association with a fracture line or between different bone segments with a bony in-growth and/or through growth region extending across the fracture line or space between different bone segments.

FIG. 6 is a front plan view of an alternative embodiment of a bone fixation/fusion device having a bony in-growth and/or bony through-growth region, in which the device has a conical configuration.

FIG. 7 is front plan view of an alternative embodiment of a bone fixation/fusion device having a bony in-growth and/or through-growth region in which the device has a beveled distal tip.

FIGS. 8A and 8B are schematics illustrating the insertion of a bone fixation/fusion device of the type shown in FIG. 6 in association with a fracture line or between different bone segments.



FIG. 9 is a schematic illustrating a guidewire being introduced into bone in association with a fracture line or between different bone segments.

FIG. 10 is a schematic similar to FIG. 9 and illustrating a drill bit being introduced over the guidewire.

FIG. 11 is a schematic similar to FIG. 10 and illustrating a bore formed in the bone remaining after withdrawal of the drill bit.

FIG. 12 is a schematic similar to FIG. 11 and illustrating insertion of a bone fixation/fusion device into the pre-formed bore.

FIG. 13 is an exploded front plan view illustrating the coupling of a pair of bone fixation/fusion by threaded engagement.

FIG. 14 is a schematic illustrating a pair of bone fixation/fusion devices coupled together and inserted in association with a fracture line or between different bone segments.

FIG. 15 is a front plan view illustrating passage of a bone fixation/fusion device through a fenestration in another bone fixation/fusion device.

FIG. 16 is a schematic illustrating the placement of a series of bone fixation/fusion devices in bone.

FIG. 17 is a top plan view of a bone fixation/fusion device positioned in association with a fracture line or between different bone segments.

FIG. 18A is a perspective view of an alternative embodiment of a bone fixation/fusion device having a bony in-growth and/or bony through-growth region that extends substantially along the entire device.

FIG. 18B is a perspective view of a bone fixation/fusion device similar to FIG. 18A and having a bony in-growth and/or bony through-growth region that extends along a portion of the device.

FIG. 19 is a top plan view of the bone fixation/fusion device of FIG. 18A in positioned in association with a fracture line or between different bone segments.

FIG. 20 is a top plan view of the bone fixation/fusion device of FIG. 18A positioned in association with a fracture line or between different bone segments and stabilized by fixation screws.

FIGS. 21A to 21F are perspective views illustrating alternative configurations of bone fixation/fusion devices of a type shown in FIG. 18A.

FIGS. 22A and 22B are perspective views illustrating alternative embodiments of the bone fixation/fusion of a type shown in FIG. 18A in which the device is profiled.

FIGS. 23A and 23B are perspective views illustrating alternative embodiments of the bone fixation/fusion device of a type shown in FIG. 1 with structural elements that provide an anti-rotational function.

FIG. 24 is a perspective view illustrating an alternative embodiment of the bone fixation/fusion device of a type shown FIG. 18A in which the device includes a series of grooves providing an anti-rotational function.

FIG. 25 is a perspective view illustrating an alternative embodiment of the bone fixation/fusion device of a type shown in FIG. 18A in which the device includes a pair of opposing wings providing an anti-rotational function.

FIG. 26 is a perspective view illustrating an alternative embodiment of the bone fixation/fusion device of FIG. 18A in which the device includes a pair of opposing flanges providing an anti-rotational function.

FIG. 27 is an exploded view of a pair of coupled bone fixation/fusion devices that, when fitted together, form a composite bone fixation/fusion device.

FIG. 28 is an assembled view of the composite bone fixation/fusion device formed from the assembly of the bone fixation/fusion devices shown in FIG. 27.

FIG. 29 is a front view of the assembled composite bone fixation/fusion device of FIG. 28 positioned in association with a fracture line or between different bone segments.

FIG. 30 is a perspective view of an alternative embodiment of the bone fixation/fusion device of a type shown in FIG. 18A with fixation plates.

FIG. 31 is a perspective view of an alternative embodiment of the bone fixation/fusion device of FIG. 30.

FIG. 32 is a side view of an alternative embodiment of a fixation plate having a rounded configuration.

FIG. 33 is a side view of an alternative embodiment of a fixation plate having a tapered configuration.

FIG. 34 is a perspective view of an alternative embodiment of the bone fixation/fusion device of a type shown in FIG. 18A providing a series of radially-extending fixation ridges.

FIGS. 35A and 35B are perspective views of a bone fixation/fusion device having a malleable region that can be flared or expanded to provide fixation and/or anti-rotation resistance.

FIG. 36 is a front plan view illustrating the drilling of pilot holes in adjacent bone segments, which can comprise a fracture line in the same bone or different bone segments.

FIG. 37 is a front plan view illustrating a cavity bored between the pilot holes to receive a bone fixation/fusion device.

FIG. 38 is a front plan view illustrating the placement of a pair of guide pins within the bored cavity.

FIG. 39 is a front plan view illustrating the placement of the bone fixation/fusion device into the cavity and removal of the guide pins.

FIG. 40 is a front plan view illustrating the placement of a pair of opposing c-shaped restraints within the bored cavity.

FIG. 41 is a front plan view illustrating the placement of the bone fixation/fusion device into the cavity within the restraints.

#### DETAILED DESCRIPTION

Although the disclosure hereof is detailed and exact to enable those skilled in the art to practice the invention, the physical embodiments herein disclosed merely exemplify the invention that may be embodied in other specific structure. While the preferred embodiment has been described, the details may be changed without departing from the invention, which is defined by the claims.

FIGS. 1A and 1B show representative alternative configurations of a device 10 sized and configured for the fixation of bone fractures (i.e., fixation of parts of the same bone) or for the fixation of bones which are to be fused (arthrodesed) (i.e. fixation of two or more individual bones that are adjacent and/or jointed). For the sake of shorthand, the device will sometimes be called a bone fixation/fusion device, to indicate that it can perform a fixation function between two or more individual bones), or a fusion function between two or more parts of the same bone, or both functions. As used herein, "bone segments" or "adjacent bone regions" refer to either situation, i.e., a fracture line in a single bone or a space between different bone segments.

In the embodiments shown in FIGS. 1A and 1B, the bone fixation/fusion device 10 comprises an elongated, stem-like structure. The device 10 can be formed—e.g., by machining, molding, or extrusion—from a material usable in the pro-

thetic arts, including, but not limited to, titanium, titanium alloys, tantalum, chrome cobalt, surgical steel, or any other total joint replacement metal and/or ceramic, sintered glass, artificial bone, any uncemented metal or ceramic surface, or a combination thereof. Alternatively, the device **10** may be formed from a suitable durable biologic material or a combination of metal and biologic material, such as a biocompatible bone-filling material. The device **10** may be molded from a flowable biologic material, e.g., acrylic bone cement, that is cured, e.g., by UV light, to a non-flowable or solid material.

The bone fixation/fusion device **10** can take various shapes and have various cross-sectional geometries. The device **10** can have, e.g., a generally curvilinear (i.e., round or oval) cross-section—as FIG. **1A** shows—or a generally rectilinear cross section (i.e., square or rectangular or triangular—as FIG. **1B** shows for purposes of illustration), or combinations thereof. As will be described in greater detail later (see, e.g., FIGS. **21A** to **21F**), instead of being shaped like an elongated stem, the body of the bone fixation/fusion device **10** can be less elongated and form more of a flattened, “wafer” configuration, having, e.g., a rectangular, square, or disc shape.

As FIGS. **2** and **3** shows, the bone fixation/fusion device **10** desirably includes a region **12** formed along at least a portion of its length to promote bony in-growth onto or into surface of the device **10** and/or bony growth entirely through all or a portion of the device **10**.

The region **12** can comprise, e.g., through holes, and/or various surface patterns, and/or various surface textures, and/or pores, or combinations thereof. The device **10** can be coated or wrapped or surfaced treated to provide the bony in-growth or through-growth region **12**, or it can be formed from a material that itself inherently possesses a structure conducive to bony in-growth or through-growth, such as a porous mesh, hydroxyapatite, or other porous surface. The device **10** may further be covered with various other coatings such as antimicrobial, antithrombotic, and osteoinductive agents, or a combination thereof. The region **12** may be impregnated with such agents, if desired.

The configuration of the region **12** can, of course, vary. By way of examples, FIG. **1** shows the region **12** as an open mesh configuration; FIG. **2** shows the region **12** as beaded configuration; and FIG. **3** shows the region **12** as a trabecular configuration. Any configuration conducive to bony in-growth and/or bony through-growth will suffice.

In use (see FIGS. **4** and **5**), the bone fixation/fusion device **10** is inserted into a space between two adjacent bone surfaces, e.g., into a fracture site in a single bone or between two bones (e.g., adjacent vertebral bodies) which are to be fused together. In FIG. **4**, the device **10** is shown being tapped into bone through bone segments **14** (i.e., across a fracture line or between adjacent bones to be fused) with a tap **16**. The bone may be drilled first to facilitate insertion of the device **10**. The bony in-growth or through-growth region **12** along the surface of the device **10** accelerates bony in-growth or through-growth onto, into, or through the device **10**. Bony in-growth or through-growth onto, into, or through the device **10** helps speed up the fusion process or fracture healing time.

The bony in-growth or through-growth region **12** may extend along the entire outer surface of the device **10**, as shown in FIG. **4**, or the bony in-growth or through-growth region **12** may cover just a specified distance on either side of the bone segments or fracture line, as shown in FIG. **5**.

The size and configuration of the device can be varied to accommodate the type and location of the bone to be treated as well as individual anatomy.

As FIG. **6** shows, the device **10** can be angled or tapered in a conical configuration. The degree of angle can be varied to accommodate specific needs or individual anatomy. A lesser degree of angle (i.e., a more acute angle) decreases the risk of splitting the bone as the device **10** is tapped into the bone or the fracture segments **14**. The device **10** may also include a beveled distal tip **18** to further add in insertion of the device **10** into bone, as shown in FIG. **7**. As shown in FIGS. **8A** and **8B**, the conical shape also helps drive the bone segments or fracture fragments together, reducing the gap (**G**) between the bone segments **14** or fracture segments.

In FIGS. **9** to **12**, the device **10** is cannulated, having a central lumen or throughbore **20** extending through it, to assist in the placement of the device **10** within bone. FIG. **1B** also shows a cannulated throughbore in a different configuration.

In use, the physician can insert a conventional guide pin **22** through the bone segments **14** by conventional methods, as FIG. **9** shows. A cannulated drill bit **24** can then be introduced over the guide pin **22**, as seen in FIG. **10**. A single drill bit or multiple drill bits **24** can be employed to drill through bone fragments or bone surfaces to create a bore **26** of the desired size and configuration. In the illustrated embodiment, the drill bit **24** is sized and configured to create a conical bore **26** similar in size and configuration to the device **10**. The bore **26** is desirably sized and configured to permit tight engagement of the device **10** within the bore **26** and thereby restrict movement of the device **10** within the bore **26**. The pre-formed bore **26** may be slightly smaller than the device **10**, while still allowing the device **10** to be secured into position within the bore **26** by tapping. As seen in FIG. **11**, the drill bit **24** is then withdrawn. The device **10** is then inserted into the bore **26** over the guide pin **22**, as FIG. **12** shows. The guide pin **22** is then withdrawn.

Alternatively, the bone fixation/fusion device **10** itself can include screw-like threads along the body for screwing the device into place. In the arrangement, the device **10** is self-tapping. Also in this arrangement, the device **10** can be cannulated for use with a guide pin **22**, or it need not be cannulated.

Multiple devices **10** may be employed to provide additional stabilization. While the use of multiple devices **10** will now be described illustrating the use of multiple devices **10** of the same size and configuration, it is contemplated that the devices **10** may also be of different size and/or configuration, e.g., one device **10** is of a cylindrical configuration and a second device **10** is of a conical configuration.

In many cases, it may be desirable to couple a series of devices **10** together, e.g., to provide stabilization over a larger surface area. A series of devices **10** may be coupled together by any suitable means, e.g., by a snap fit engagement, or a groove and tab key arrangement, or by a Morse taper fit, or combinations thereof. In one embodiment, a series of devices **10** are coupled by threaded engagement. As illustrated in FIG. **13**, a first device **10A** includes a recess **28** at one end providing a series of internal threads **30**. In the illustrated embodiment, the first device **10** is of a cylindrical configuration, but may be of any desired configuration. The internal threads **30** couple with a series of complementary external threads **32** on a second device **10B** of a similar or of a different configuration to couple the first and second devices **10A** and **10B** together.

The devices **10A** and **10B** are desirably coupled together prior to being inserted into the pre-formed bore **26**. The

series of internal and external threads **30** and **32** provide an interlocking mechanism that permits a series of devices **10** to be stacked and connected to cover a larger area or multiple bone segments **14** (e.g., a bone having multiple fractures) and thereby provides additional stabilization, as seen in FIG. **14**.

FIG. **15** illustrates another embodiment in which a device **10'** includes an opening or fenestration **34** to allow another device **10** to pass through, thereby providing additional stabilization. The fenestration **34** can be sized and configured to permit another device **10** to be passed through the device **10'** at virtually any angle. The fenestration **34** can also be sized and configured to limit movement of the second device **10** relative to the second device **10'**.

In use, and as shown in FIG. **16**, the physician taps a first device **10'** having a fenestration **34** through the bone segments. A second device **10** is then inserted (e.g., by tapping) through the fenestration **34** of the first device **10'** into place.

It is further contemplated that device **10'** may also be adapted for coupling with another device **10A** (e.g., by a series of external and internal threads), permitting the devices **10'** and **10A** to be additionally stacked and connected, as also shown in FIG. **16**.

FIG. **17** illustrates an alternative form of a bone fixation/fusion device **100**. Similar to the type of bone fixation/fusion device **10** previously described, device **100** includes a body **106** formed of a durable material that is not subject to significant bio-absorption or resorption by surrounding bone or tissue over time. In other words, the body **106** is intended to remain in place for a time sufficient to stabilize the fracture or fusion site. Such materials are well known in the prosthetic arts and include, e.g., titanium, titanium alloys, tantalum, chrome cobalt, surgical steel, or any other total joint replacement metal and/or ceramic, sintered glass, artificial bone, any uncemented metal or ceramic surface, or a combination thereof. Alternatively, the body **106** of the bone fixation/fusion device **100** may be formed from a suitable durable biologic material or a combination of metal and biologic material, such as a biocompatible bone-filling material. The body **106** of the device **100** may be molded from a flowable biologic material, e.g., acrylic bone cement, that is cured, e.g., by UV light, to a non-flowable or solid material.

The body **106** of the device **100** may also include a bony in-growth or through-growth region **108**, as already described in association with previous embodiments.

Unlike the bone fixation/fusion device **10**, the bone fixation/fusion device **100** includes at least one region associated with the body **106** that, in contrast to the body **106**, comprises a material that is subject to more rapid in vivo bio-absorption or resorption by surrounding bone or tissue over time, e.g., within weeks or a few months. The resorbable material can comprise, e.g., polylactic acid (PLA), polyglycolic acid (PGA), poly(lactideglycolide) copolymers, polyanhydrides, cyclode, cirnsns, polyorthoesters, n-vinyl alcohol, or other biosorbable polymers or like materials known or recognized in the prosthetic arts as having such characteristics. The bio-absorbable region is intended to facilitate implantation or placement of the body **106**, but over time be absorbed to minimize the footprint of the implanted device **100** in the long run.

The bioabsorbable region or regions can possess functionality to aid in the implantation process. For example, as shown the illustrated embodiment, there are two bioabsorbable regions **102** and **104**. Region **102** comprises a bioabsorbable screw region **102**, which is desirably threaded or otherwise suitably configured to pierce bone and facilitate

advancement of the device **100** into bone. The other region **104** comprises a bioabsorbable head region **104**, which is desirably configured to mate with an installation instrument, (e.g., a screwdriver, to further facilitate advancement and positioning of the bone fixation/fusion device **100** in the bone. The bioabsorbable head **104** may also be sized and configured to temporarily anchor the device **100** within bone, e.g., the head **104** may be a slightly larger diameter than the body **106** of the device **100**. The bioabsorbable screw portion **102** and head portion **104** are configured to provide an immediate benefit during the initial placement or position of the device **100**, but over time be resorbed when they have served their initial purpose during implantation. This leaves the more durable and less resorbable body **106** behind, to serve its longer-term function of stabilizing the fracture or fusion site.

As previously disclosed, a given bone fixation/fusion device can take various shapes and geometries. For example, as shown in FIGS. **18A** and **18B**, the bone fixation/fusion device **200** possesses a flattened rectangular (or wafer-like) configuration. A region **12** of the device **200** can be textured or treated, as previously described, to provide bony in-growth or through-growth. The bony in-growth or through-growth region **12** may extend along the entire device **200** (see FIG. **18A**) or along any portion or portions of the device **200** (see FIG. **18B**).

The bone fixation/fusion device **200** is desirably sized and configured to be positioned to join two or more adjacent bone segments **14** (which can comprise a fracture site, a fusion site, or both), as FIG. **19** shows, to fix and to promote the fusion of the adjacent bone segments **14**. The device **200** may also be sized and configured to fix and to promote fusion of multiple bone segments **14** or compound fractures, as FIG. **20** shows. FIG. **20** illustrates placement of the bone fixation/fusion device **200** sized and configured for the fixation and fusion of, for example, a first cuneiform (CE1), a second cuneiform (CE2), a first metatarsal (M1), and a second metatarsal (M2).

As shown in FIG. **20**, one or more auxiliary fixation elements, such as conventional orthopedic screws **206**, may also be placed within and/or across the bone segments **14** by conventional techniques, to augment the stabilization of the bone segments **14** during the fusion process.

The size and configuration of the bone fixation/fusion device **200** may be modified or adjusted in diverse ways to serve the intended stabilization function in diverse bone locations, bone geometries, or bone types, which are intended to be fused or repaired. The bone fixation/fusion device **200** can come in a family of different pre-established sizes and shapes, or it can be individually sized and configured to meet the requirements of a particular individual's anatomy. For the sake of illustration, by not limitation, a given bone fixation/fusion device **200** may take the form of a disc (FIG. **21A**), a square (FIG. **21B**), or an oval (FIG. **21C**). The height, width, and length of a given bone fixation/fusion device **200** may be varied depending on the specific location and amount of bone to be crossed for stabilization. A given bone fixation/fusion device may possess a symmetric geometry, or an asymmetric or complex geometry—such as an L shape (FIG. **21D**), a triangle (FIG. **21E**), or rectangle with a triangular ends (FIG. **22F**). Any combination of linear or curvilinear or rounded geometries is possible.

As before described, a given bone fixation/fusion device can be cannulated to aid in guidance during placement or implantation. For example, as shown in FIGS. **18A** and **18B**, the device **200** can include a pair of opposing guide bores **202**. The guide bores **202** are sized and configured to

accommodate passage of guide pins **204**, which are secured at the intended site of fixation/fusion device **200** can be guided by the pins **204** to the intended bone placement site.

To aid in stabilizing a given bone fixation/fusion device within bone, the device may be profiled. For example, as shown in FIG. **22A**, the bone fixation/fusion device **200** may vary in height across its entire length of the device **200**, to form a tapered wedge. Alternatively, as shown in FIG. **22B**, the bone fixation/fusion device **200** may vary in height at one end only. In these arrangements, the bone fixation/fusion device **200** is desirably positioned with the area of greatest height in the proximal direction, which serves to wedge the device **200** into place within bone.

To also aid in stabilizing a given bone fixation/fusion device within bone, the device can include one or more anti-rotational elements, which further stabilize and secure the device in the desired position within bone. The size and configuration of the anti-rotational elements may vary. For example, the anti-rotational elements may comprise an array of fins **300** projecting from a stem-like device **10** (FIG. **23A**), or an array of grooves **302** formed in a rectangular wafer device **200** (FIG. **24**), or wings **304** formed in a rectangular wafer device **200** (FIG. **25**), or flanges **306** projecting from a wafer device **200** (FIG. **26**). The anti-rotational elements can comprise (see FIG. **23B**) an array of bumps **308** or surface projections **310** formed on all or a portion of the device, which can be either stem-like or wafer-like in its configuration. Any number of anti-rotational elements, or any configuration of anti-rotational elements, or any combinations of configurations can be provided to serve the functional objective of stabilization.

As also previously described, two or more bone fixation/fusion devices **200** of the types generally described above may be assembled to form a composite bone fixation/fusion device having a desired size and configuration. For example, in the arrangement shown in FIGS. **27** to **29**, the bodies of two bone fixation/fusion devices **200** each have a slot **208**. Slot **208** in a first device **200** mates with a like or complementary slot **208** in a second device **200** to permit the assembly of a composite bone fixation/fusion device **310**, which has a crossed, anti-rotational configuration for placement across bone segments **14**. The crossed relation of the composite bone fixation/fusion device **310** has an increased surface area and adds further stability to the devices **200** in bone during the fusion process.

It will be apparent to one of skill in the art that the location, size, and configuration of the slots **208** may be varied to accommodate specific needs and a specific anatomical location as well as individual anatomy. It is also apparent that other mating configurations, e.g., groove and tab fits, or snap-fit arrangements, or Morse taper fits, or threaded assemblies, can be used to assemble two or more bone fixation/fusion devices into a composite device **310**.

As shown in FIGS. **30**, fixation or gripping plates **212** may be fitted to a given bone fixation/fusion device. In the arrangement shown in FIG. **30**, the body of the bone fixation/fusion device **200** includes one or more attachment sites **210**, e.g., slits or indentations, which are sized and configured to receive a selectively removable fixation or gripping plate **212**. When received within the slit **210**, the plate **212** extends radially from the device to grip into bone and further secure the device **200** within bone.

In an alternative embodiment, shown in FIG. **31**, the attachment site **210** can include a tab **214**, which mates with a notch **216** in the fixation plate **212** to secure the plate **212** within the device **200**.

Other forms of interlocking or nesting configuration can be used. For example, tongue-and-groove fitments, or snap-fit arrangements, or threaded fitments, or Morse taper assemblies can be used to assemble one or more fixation or gripping plates to a bone fixation/fusion device.

The fixation or gripping plate **212** is formed of durable biocompatible metal or bone substitute material, as previously described. In some cases, it may be desirable to provide a bony in-growth surface on at least a portion of the plate **212**. Alternatively, the plate **212** may be formed of a bio-absorbable material, as already described.

FIGS. **30** and **31** illustrate embodiments in which the plates **212** present a generally blunt and flat configuration. It will be apparent to one of skill in the art that, however, that the plates **212** may also provide a sharpened or cutting edge or be otherwise sized and configured as necessary to accommodate specific location and individual anatomy. For example, the plate **212** may be rounded (FIG. **32**) or tapered (FIG. **33**).

FIG. **34** illustrates an alternative embodiment in which one or more fixation ridges **218** extend radially from the bone fixation/fusion device **200**. Similar to the fixation plates **212**, the ridges **218** may be variously sized and configured so as to grip into bone and further secure the bone fixation/fusion device **200** within bone.

Fixation elements can be formed in situ. For example, as shown in FIG. **35A**, a bone fixation/fusion device **200** can include a malleable region **320** that normally presents a low-profile conducive to implantation. As FIG. **35B** shows, the profile of the malleable **320** can be changed in situ after implantation to a radially enlarged or extended profile **326** that provides stabilization or an anti-rotational function to the device **200**. In the illustrated embodiment, the malleable region **320** is slotted (see FIG. **35A**) to accommodate placement of a wedge tool **324** carried for manipulation by a stylet or cannula **322** (see FIG. **35B**). The wedge tool **324** flays apart the slotted malleable region **320** (as FIG. **35B** shows), to create the enlarged profile **326** for stabilization and/or rotation resistance.

In use, and with reference to FIG. **36**, pilot holes **220** are drilled into adjacent bone segments **14** (e.g., along a fracture line in a single bone or between adjacent segments of different bones) by conventional surgical techniques. In the illustrated embodiment, a single pilot hole **220** is drilled into each bone segment **14**. It is to be understood that the number and configuration of the pilot holes **220** may vary as necessary or as desired.

As shown in FIG. **37**, the physician can then then saw, using conventional methods, between the pilot holes **220** to prepare a cavity **222** to receive the device **200**.

Guide pins **204** may, if desired, be placed at opposing ends of the bored cavity **222**, as seen in FIG. **38**. In this arrangement, as shown in FIG. **39**, the selected bone fixation/fusion device **200** is passed over the guide pins **204** to position the device **200** with the cavity **222**. The guide pins **204** may then be removed. In an alternative arrangement, guide pins **204** need not be used, and the device **200** is manually inserted by the physician into the bore cavity **222**.

An alternative embodiment is illustrated in FIGS. **40** and **41**. In this embodiment, a c-shaped restraint **224** is placed against each end of the bored cavity **222**. The selected bone fixation/fusion device **200** is then positioned between the restraints **222** such that the restraints **222** engage the device **200** to secure the device **200** within bone.

The foregoing is considered as illustrative only of the principles of the invention. Furthermore, since numerous modifications and changes will readily occur to those skilled

11

in the art, it is not desired to limit the invention to the exact construction and operation shown and described. While the preferred embodiment has been described, the details may be changed without departing from the invention, which is defined by the claims.

What is claimed is:

1. A method comprising:  
 identifying a bone site comprising a first bone segment, a second bone segment, and a joint between the first and second bone segments;  
 providing an elongated bone fusion device having a longitudinal axis and a rectilinear cross section transverse to the longitudinal axis and including an exterior surface treated to provide bony in-growth;  
 forming a bore having a longitudinal axis in the first bone segment;  
 forming a bore having a longitudinal axis in the second bone segment that faces the bore in the first bone segment across the joint, the bores in the first and second segments each being non-parallel to the joint and having a rectilinear cross-sectional profile sized and configured to tightly engage the exterior surface of the elongated bone fusion device, wherein the rectilinear cross-sectional profile of each bore is transverse to the longitudinal axis of each bore; and  
 fusing the joint by inserting the elongated bone fusion device across the joint and into tight engagement within the bores of the first and second bone segments, to thereby restrict movement of the elongated bone fusion device across the joint and provide bony in-growth within the bores along the exterior surface of the bone fusion device.
2. A method according to claim 1, wherein the rectilinear cross section of the elongated bone fusion device comprises a square.
3. A method according to claim 1, wherein the rectilinear cross section of the elongated bone fusion device comprises a rectangle.
4. A method according to claim 1, wherein the rectilinear cross section of the elongated bone fusion device comprises a triangle.

12

5. A method according to claim 1, wherein forming the bore in the first bone segment comprises drilling a pilot bore with a drill bit.
6. A method according to claim 1, wherein inserting the elongated bone fusion device across the joint comprises tapping the bone fusion device.
7. A method comprising:  
 identifying a bone site comprising a first bone segment, a second bone segment, and a joint between the first and second bone segments;  
 providing an elongated bone fusion device having a longitudinal axis and a cross sectional profile transverse to the longitudinal axis that is defined by at least one apex, wherein the elongated implant structure comprises an exterior surface region treated to provide bony in-growth;  
 forming a bore having a longitudinal axis in the first bone segment;  
 forming a bore having a longitudinal axis in the second bone segment that faces the bore in the first bone segment across the joint, the bores in the first and second segments each being non-parallel to the joint and having a cross-sectional profile defined by at least one apex sized and configured to tightly engage the exterior surface of the elongated bone fusion device, wherein the cross-sectional profile defined by at least one apex of each bore is transverse to the longitudinal axis of each bore; and  
 fusing the joint by inserting the elongated bone fusion device across the joint and into tight engagement within the bores of the first and second bone segments, to thereby restrict movement of the elongated bone fusion device across the joint and provide bony in-growth within the bores along the exterior surface of the bone fusion device.
8. A method according to claim 7, wherein the cross sectional profile is defined by three apices.
9. A method according to claim 7, wherein the cross sectional profile is defined by four apices.
10. A method according to claim 7, wherein inserting the elongated bone fusion device across the joint comprises tapping the bone fusion device.

\* \* \* \* \*