



(19) **United States**

(12) **Patent Application Publication**

Eder et al.

(10) **Pub. No.: US 2013/0219620 A1**

(43) **Pub. Date: Aug. 29, 2013**

(54) **PATIENT SUPPORT APPARATUS AND MEDICAL IMAGING APPARATUS HAVING THE PATIENT SUPPORT APPARATUS**

Publication Classification

(71) Applicants: **Hanns Eder**, Bubenreuth (DE); **Patrick Gross**, Langensendelbach (DE); **Martin Requardt**, Nurnberg (DE); **Martin Ringholz**, Erlangen (DE); **Markus Schmidt**, Nuernberg (DE)

(51) **Int. Cl.**
A61B 6/04 (2006.01)
A61G 7/00 (2006.01)
(52) **U.S. Cl.**
CPC *A61B 6/0407* (2013.01); *A61G 7/00* (2013.01)
USPC *5/601*; *5/600*

(72) Inventors: **Hanns Eder**, Bubenreuth (DE); **Patrick Gross**, Langensendelbach (DE); **Martin Requardt**, Nurnberg (DE); **Martin Ringholz**, Erlangen (DE); **Markus Schmidt**, Nuernberg (DE)

(57) **ABSTRACT**

A patient support apparatus is provided. The patient support apparatus has a patient table, a movable support plate for supporting a patient, a guide unit, which is designed to guide the support plate along at least one movement direction of the support plate, and a fastening unit for fastening an auxiliary unit to the support plate. The fastening unit has at least one setting unit for setting the position of the auxiliary unit in relation to the support plate in a flexible manner.

(21) Appl. No.: **13/775,497**

(22) Filed: **Feb. 25, 2013**

(30) **Foreign Application Priority Data**

Feb. 29, 2012 (DE) 102012203119.7

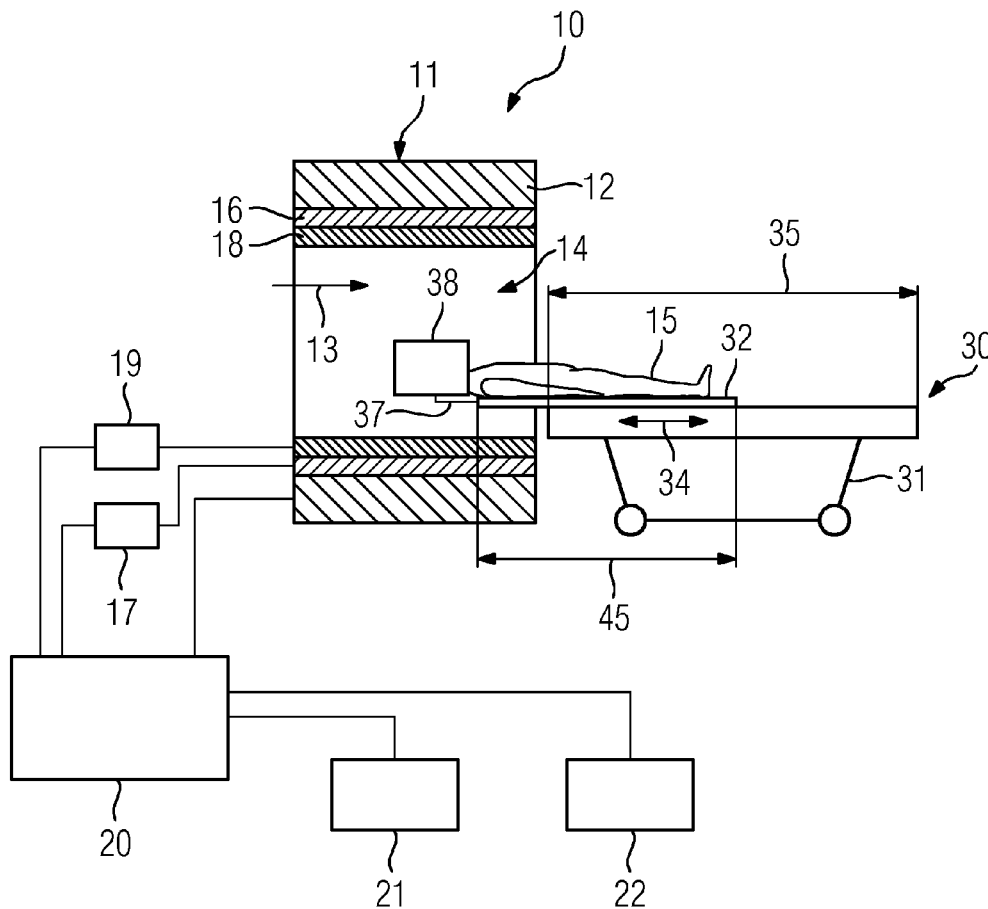


FIG 1


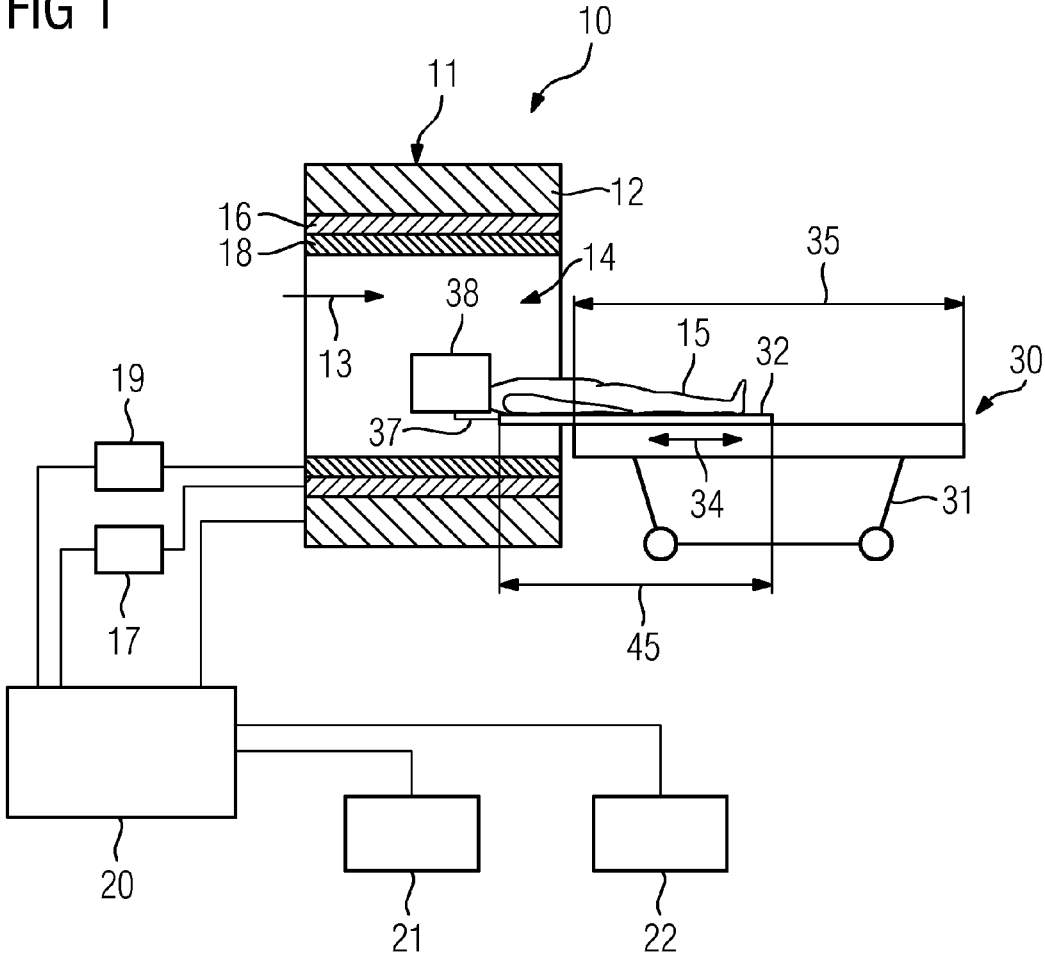


FIG 2

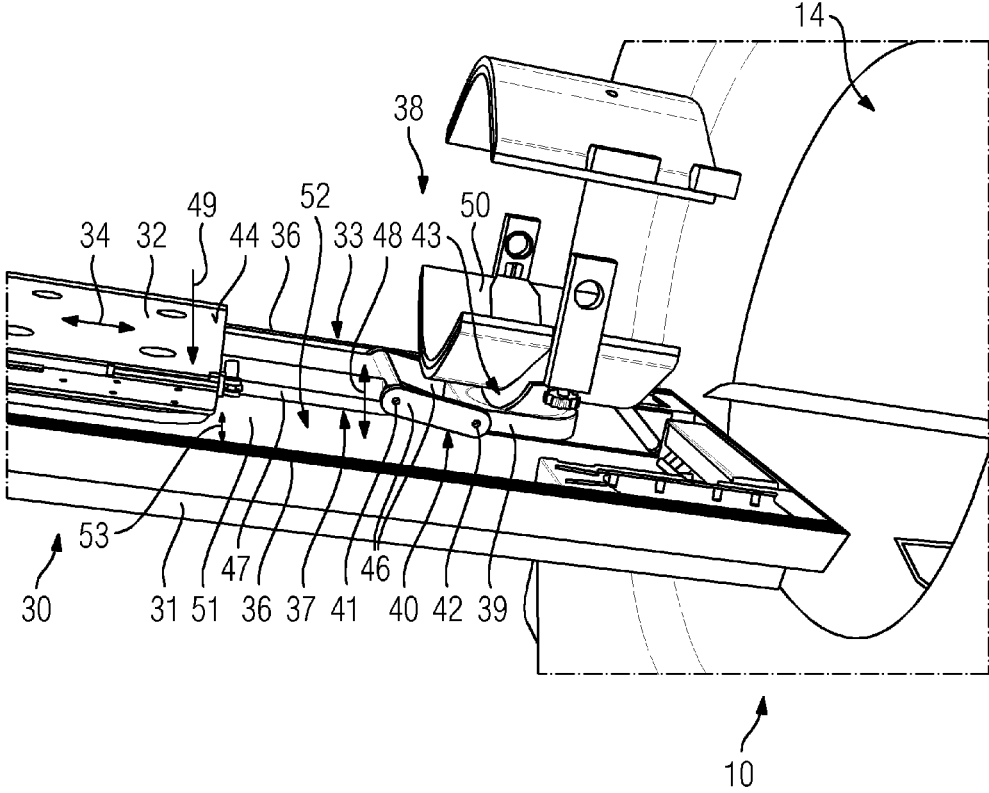

**PATIENT SUPPORT APPARATUS AND
MEDICAL IMAGING APPARATUS HAVING
THE PATIENT SUPPORT APPARATUS**

**CROSS REFERENCE TO RELATED
APPLICATIONS**

[0001] This application claims priority of German application No. 10 2012 203 119.7 filed Feb. 29, 2012, which is incorporated by reference herein in its entirety.

FIELD OF INVENTION

[0002] The present application relates to a patient support apparatus having a patient table, a movable support plate for supporting a patient, a guide unit, which is designed to guide the support plate along at least one movement direction of the support plate, and a fastening unit for fastening an auxiliary unit to the support plate.

BACKGROUND OF INVENTION

[0003] Previous patient support apparatuses have a patient table and a support plate for supporting a patient. This support plate is supported in such a manner that it can be moved by a guide unit along a longitudinal extension of the patient support apparatus. The patient support apparatus also has a fastening unit for fastening a head coil unit to the support unit. The head coil unit here is fastened to a contact surface of the support unit.

SUMMARY OF INVENTION

[0004] The object underlying the present application is to provide a patient support apparatus, which allows flexible support and/or fastening of an auxiliary unit in different positions in respect of the support unit. The object is achieved by the features of the independent claims. Embodiments are set out in the dependent claims.

[0005] The application is based on a patient support apparatus having a patient table, a movable support plate for supporting a patient, a guide unit, which is designed to guide the support plate along at least one movement direction of the support plate, and a fastening unit for fastening an auxiliary unit to the support plate.

[0006] It is proposed that the fastening unit has at least one setting unit for setting the position of the auxiliary unit in relation to the support plate in a flexible manner. The auxiliary unit can be disposed in different positions in relation to the support unit. The auxiliary unit is formed by a coil unit, such as a head coil unit, so that the patient, such as the head region of the patient, can be supported in a position desired by an operator and/or in a support position appropriate for the anatomy of the patient. The disclosed patient support apparatus is configured for use in conjunction with a medical imaging apparatus. The integration of the auxiliary unit, such as the head coil unit, on the support plate of the patient support apparatus means that the disclosed patient support apparatus is suitable for a medical imaging apparatus formed by a magnetic resonance apparatus. The movable support plate means that the patient support apparatus can be provided for examinations during or after an intervention by a physician, such as a surgical intervention in a head region of the patient. The patient can remain lying on the support plate and is picked up from an operating table together with the support plate by the patient support apparatus and moved for example to the magnetic resonance apparatus, with the support plate

being moved, after the two patient support apparatuses have been docked, from the first patient support apparatus to the second patient support apparatus by the guide unit. As a magnetic resonance examination is frequently used to monitor or continue the surgical intervention, the head of the patient is fixed within the head coil unit during this process, with the head also being able to offer open operating access or open intervention access. The patient support apparatus here is formed by a patient support apparatus for neurosurgical interventions, having an interface for coupling to at least one medical imaging apparatus and having at least one interface for coupling to an operating table, on which the neurosurgical interventions on the patient take place.

[0007] It is further proposed that the fastening unit is disposed on a lower face and/or on a front face of the support plate, thereby allowing a space-saving and compact patient support apparatus to be achieved. A “lower face” here refers to a face of the support plate facing away from the support surface. A “front face” here refers to a face disposed in a head support region of the support plate, which is also aligned perpendicular to a longitudinal extension of the support plate.

[0008] It is further proposed that the fastening unit has at least one subregion, which extends away from the support plate along a direction from a contact surface toward the lower face, so that the auxiliary unit, such as the head coil unit, can be disposed in an optimum position for the patient and/or the operator, in an appropriate and ergonomic position, as used for example for conventional neurosurgical support of the patient without intraoperative imaging, in relation to the support plate.

[0009] The patient support apparatus has a substructure cover, with a region for receiving the fastening unit with a height of 40 mm to 80 mm disposed between the substructure cover and a lower face of the support plate. The region has a height of 50 mm to 70 mm, allowing lowering of the head coil to be achieved during an examination and/or an intervention by a physician. A “region for receiving the fastening unit” here refers to a region between the substructure cover and the lower face of the patient couch, in which no additional units, such as coil elements, cables, etc., are disposed, so that when the support plate is displaced, the fastening unit can move freely within the region for receiving the fastening unit. To this end the region for receiving the fastening unit is of the same height along the entire longitudinal extension of the patient support apparatus.

[0010] In one development of the application it is proposed that the support plate is formed by a removable plate, so that the support plate can be used for different support apparatuses, for example in an operating support apparatus, a patient support apparatus for a medical imaging apparatus, etc. The region for receiving the fastening apparatus also allows interference-free movement of the support plate from a first support apparatus to a second support apparatus. A “removable plate” here refers to a support plate for supporting the patient, which can be moved around between different patient support apparatuses. To this end the patient support apparatuses have guide units with slide elements, so that the support plate can be switched without interference and with little friction from a first patient support apparatus to a second patient support apparatus, with the two patient support apparatuses docking with one another for the support plate switch.

[0011] It is further proposed that the at least one setting unit has at least one articulation unit for moving and/or setting the position of the auxiliary unit, such as the head coil unit, along

at least one spatial direction. This allows the setting of the position of the head coil unit and/or of the head region of the patient to be adjusted in a flexible manner. The setting unit can also have at least one articulation unit for moving and/or setting the position of the auxiliary unit, such as the head coil unit, along at least two spatial directions. Alternatively it is also conceivable for the setting unit also to have a number of articulation units for setting a position and/or movement of the head coil unit. It is thus possible to achieve setting of the position of the auxiliary unit, such as the head coil unit, along a number of spatial directions and thus to adjust the position of the auxiliary unit, such as the head coil unit, to the anatomy of the patient and/or to an optimum treatment position for surgical intervention for example at the head region of the patient. The articulation units here can have a rotary articulation and/or a ball articulation and/or further articulation units that appear expedient to the person skilled in the art. The fastening unit also has a holding region for holding the auxiliary unit, such as the head coil unit.

BRIEF DESCRIPTION OF THE DRAWINGS

[0012] Further features and details of the application will emerge from the embodiment described in the following and with reference to the drawings, in which:

[0013] FIG. 1 shows a schematic diagram of a disclosed medical imaging apparatus and

[0014] FIG. 2 shows a disclosed patient support apparatus.

DETAILED DESCRIPTION OF INVENTION

[0015] FIG. 1 shows a schematic diagram of a disclosed medical imaging apparatus, formed in the present embodiment by way of example by a magnetic resonance apparatus 10. However the embodiment of the medical imaging apparatus is not restricted to the magnetic resonance apparatus 10; the medical imaging apparatus can of course also be formed by a computed tomography apparatus, a PET apparatus, a mobile or fixed x-ray-based C-arm system, a SPECT apparatus, etc.

[0016] The magnetic resonance apparatus 10 comprises a magnetic unit 11 with a main magnet 12 for generating a powerful and constant main magnetic field 13. The magnetic resonance apparatus 10 also has a cylindrical receiving region 14 for receiving a patient 15, the receiving region 14 being enclosed in a peripheral direction by the magnetic unit 11. The patient 15 can be introduced by a patient support apparatus 30 of the magnetic resonance apparatus 10 into the receiving region 14. To this end the patient support apparatus 30 is configured in a movable manner.

[0017] The magnetic unit 11 also has a gradient coil 16 for generating magnetic field gradients, which is used for spatial encoding during imaging. The gradient coil 16 is controlled by a gradient control unit 17. The magnetic unit 11 also has a cylindrical high-frequency coil unit 18 and a high-frequency control unit 19 for stimulating polarization, which is established in the main magnetic field 13 generated by the main magnet 12. The high-frequency coil unit 18 is controlled by the high-frequency control unit 19 and emits high-frequency magnetic resonance sequences into an examination space, which is formed by the receiving region 14. This deflects the magnetization from its equilibrium position. Magnetic resonance signals are also received by the high-frequency coil unit 18.

[0018] To control the main magnet 12, the gradient control unit 17 and to control the high-frequency control unit 19, the magnetic resonance apparatus 10 has a control unit 20 formed by a computation unit. The computation unit controls the magnetic resonance apparatus 10 centrally, for example the performance of a predefined imaging gradient echo sequence. Control information, such as imaging parameters for example, and reconstructed magnetic resonance images can be displayed to an operator on a display unit 21, for example on at least one monitor, of the magnetic resonance apparatus 10. The magnetic resonance apparatus 10 also has an input unit 22, by which information and/or parameters can be input by an operator during a measuring operation.

[0019] The illustrated magnetic resonance apparatus 10 can of course comprise further components that are normally a feature of magnetic resonance apparatuses 10. A general mode of operation of a magnetic resonance apparatus 10 is also known to the person skilled in the art so there is no need for a detailed description of the general components here.

[0020] The patient support apparatus 30 is shown in more detail in FIG. 2. For use with the magnetic resonance apparatus 10 the patient support apparatus 30 is configured as magnetic resonance-compatible. The patient support apparatus 30 is formed by a patient support apparatus 30 for neurosurgical interventions having an interface for coupling to at least one medical imaging apparatus, such as a magnetic resonance apparatus 10, and having at least one interface for coupling to an operating table (not shown in detail).

[0021] The patient support apparatus 30 has a table 31 and a movable support plate 32 for supporting the patient 15. The patient support apparatus 30 also has a guide unit 33, which is designed to guide the support plate 32 along a movement direction 34 of the support plate 32. The movement direction 34 here is aligned parallel to a longitudinal extension 35 of the patient support apparatus 30.

[0022] The guide unit 33 has two guide rails 36, each disposed on a side peripheral region of the table 31 along the longitudinal extension 35 of the patient support apparatus 30. The guide rails 36 here are provided with slide elements (not shown in detail), which can be formed by roller slide elements and/or other slide elements that appear expedient to the person skilled in the art. This allows the support plate 32 to be moved and/or guided with little friction along the longitudinal extension 35 in relation to the table 31. The support plate 32 can also have slide elements and/or guide elements (not shown in detail), such as for example guide rails, of the guide unit 33. The guide unit 33 supports the support plate 32 in such a manner that it can be moved along the longitudinal extension 35, it being possible to switch from the patient support apparatus 30 to an operating table support apparatus in the process. To this end the support plate 32 is formed by a removable plate.

[0023] The patient support apparatus 30 also has a fastening unit 37 for fastening an auxiliary unit formed by a head coil unit 38. In one alternative embodiment of the application the auxiliary unit can also be formed by further units or elements.

[0024] The fastening unit 37 has a holder 39, within which the head coil unit 39 is disposed. The fastening unit 37 is configured in such a manner that it is possible to set the position of the head coil unit 38 in relation to the support plate 32 in a flexible manner. To this end the fastening unit 37 has a setting unit 40, which comprises at least one articulation unit 41, 42, 43. In the present embodiment the setting unit 40

has three articulation units **41**, **42**, **43**. The first articulation unit **41** is formed by a first rotary articulation unit and the second articulation unit **42** is formed by a second rotary articulation unit. The first rotary articulation unit and the second rotary articulation unit are disposed parallel to one another, with a rotation axis of the first rotary articulation unit and a rotation axis of the second rotary articulation unit disposed parallel to one another. The two rotation axes are also disposed parallel to a contact surface **44** of the support plate **32** and orthogonal to a longitudinal extension **45** of the support plate **32**. The two rotary articulation units are connected to one another by way of two bars **46** disposed parallel to one another.

[0025] The first rotary articulation unit allows a rotational movement of the two parallel bars **46** about the rotation axis of the first rotary articulation unit in relation to a holding element **47** of the fastening unit **37** connected in a fixed manner to the support plate. The second rotary articulation unit allows a rotational movement of the two parallel bars **46** about the rotation axis of the second rotary articulation unit in relation to the holder **39** for arranging the head coil unit **38**. When the position of the head coil unit **38** is being set, the two rotary articulation units allow said head coil unit **38** to be displaced along the longitudinal extension **45** of the support plate **32** and along a second spatial direction **48**, which is aligned perpendicular to the longitudinal extension **45** of the support plate **32** and perpendicular to the support surface **44** of the support plate **32**.

[0026] The holder **39** for arranging the head coil unit **38** also has the third articulation unit **43** of the setting unit **40**, which comprises a rotary articulation unit. A rotation axis of said third rotary articulation unit is aligned perpendicular to the rotation axes of the first and second rotary articulation units and also perpendicular to the support surface **44** of the support plate **32**. This allows a rotation of the head coil unit **38** parallel to the support surface **44** of the support plate **32** to be achieved. The third articulation unit **43** can also produce a rotation of the head coil unit **38** within the plane aligned perpendicular to the contact surface **44** of the support plate **32**.

[0027] Alternatively or additionally the setting unit **40** and/or the individual articulation units **41**, **42**, **43** of the setting unit **40** can also be embodied differently from a rotary articulation unit. For example the articulation units **41**, **42**, **43** can also be formed by ball articulation units, rotary push-in articulation units and/or further articulation units that appear expedient to the person skilled in the art. It is also conceivable for the number of articulation units to vary, when individual articulation units can be set with a number of degrees of freedom.

[0028] The setting of the fastening unit **37**, such as of the setting unit **40**, for a desired position of the head coil unit **38** is effected manually here by an operator, for example a clinician. Alternatively or additionally at least partially automatic and/or self-activated setting of the position of the head coil unit **38** by the setting unit **40** is conceivable, for example by an electric or electronic setting unit, etc.

[0029] The fastening unit **37** is disposed on the support plate **32** of the patient support apparatus **30**. To this end the fastening unit **37** is disposed in a fixed manner with the holding element **47** on the support plate **32**, the arrangement being effected on a lower face formed by a face of the support plate **32** facing away from the support surface **44** and/or on a front face of the support plate **32**. In the present embodiment

the fastening unit **37** is disposed on the lower face of the support plate **32**. The holding element **47** of the fastening unit **37** here can be screwed, bonded or riveted to the support plate **32** and/or can be connected in a fixed manner to the support plate **32** by further fastening methods.

[0030] The arrangement of the fastening unit **37** on the lower face and/or on the front face of the support plate **32** means that the fastening unit **37** projects beyond the dimensions of the support plate **32**. The fastening unit **37** projects beyond the support plate **32** along a direction **49** from the support surface **44** toward the lower face of the support plate **32**. Depending on the position set at the fastening unit **37**, the fastening unit **37** can have a maximum extension of approx. 70 mm relative to the support plate **32** along this direction **49**. The maximum extension has a length of approx. 60 mm and a length of approx. 50 mm. The fastening unit **32** also projects beyond the front face along the longitudinal extension **45** of the support plate **32**, so that, when mounted on the fastening unit **37**, the head coil unit **38** is disposed outside the dimensions of the support plate **32** along the longitudinal extension **45** of the support plate **32**. It is possible for the head coil unit **38**, a bearing surface **50** of the head coil unit **38** for contact with the head of a patient **15**, to be lowered to and/or disposed at the height of the contact surface **44** by the fastening unit **37**, such as by the setting unit **40**.

[0031] The patient support apparatus **30**, such as the table **31**, also has a substructure cover **51**, which is designed to cover a region for receiving a controller, an electronic unit and/or further units and/or elements that appear expedient to the person skilled in the art, and which covers a face of the patient table **31** facing the support plate **32**. For interference-free movement of the support plate **32** together with the lowered head coil unit **38** relative to the substructure cover **51**, the patient support apparatus has a region **52** for receiving the fastening unit **37**, with the fastening unit **37** projecting out from the support plate **32** into said region **52**. This region **52** for receiving the fastening unit **37** has a height **53** of approx. 40 mm to approx. 80 mm, however a height **53** of 50 mm to 70 mm and a height **53** of at least 55 mm. This region **52** for receiving the fastening unit **37** has the same height **53** along the entire longitudinal extension **35** of the patient support apparatus **30**. Said region **52** also extends along an entire transverse extension between the two guide rails **36** of the table **31**, so that unwanted tilting of the fastening apparatus **37** is prevented during movement of the support plate **32** along the longitudinal extension **35**.

1. A patient support apparatus, comprising:
 - a support plate for supporting a patient;
 - a guide unit for guiding the support plate along at least one movement direction of the support plate;
 - an auxiliary unit;
 - a fastening unit for fastening the auxiliary unit to the support plate; and
 - a setting unit for flexibly setting a position of the auxiliary unit in relation to the support plate.
2. The patient support apparatus as claimed in claim 1, wherein the auxiliary unit is formed by a head coil unit.
3. The patient support apparatus as claimed in claim 1, wherein the fastening unit is disposed on a lower face and/or on a front face of the support plate.
4. The patient support apparatus as claimed in claim 3, wherein the fastening unit comprises at least one subregion that extends away from the support plate along a direction from a contact surface toward the lower face.

5. The patient support apparatus as claimed in claim 1, further comprising a substructure cover having a region for receiving the fastening unit, wherein the region has a height of 40 mm to 80 mm and is disposed between the substructure cover and a lower face of the support plate.

6. The patient support apparatus as claimed in claim 5, wherein the region has a height of 50 mm to 70 mm.

7. The patient support apparatus as claimed in claim 5, wherein the region has a same height along entire longitudinal extension of the patient support apparatus.

8. The patient support apparatus as claimed in claim 1, wherein the support plate is formed by a removable plate.

9. The patient support apparatus as claimed in claim 1, wherein the setting unit comprises at least one articulation unit for moving and/or setting the position of the auxiliary unit along at least one spatial direction.

10. The patient support apparatus as claimed in claim 1, wherein the setting unit comprises at least one articulation unit for moving and/or setting the position of the auxiliary unit along at least two spatial directions.

11. A medical imaging apparatus, comprises:

a patient support apparatus as claimed in claim 1.

12. The medical imaging apparatus as claimed in claim 11, wherein the medical imaging apparatus is a magnetic resonance apparatus.

* * * * *